



**HAL**  
open science

## Influence of probe size for local electrochemical impedance measurements

Caio G Palumbo de Abreu, Camila Molena de Assis, Patricia H. Suegama, Isolda G Costa, Michel Keddam, Hercilio G. de Melo, Vincent Vivier

► **To cite this version:**

Caio G Palumbo de Abreu, Camila Molena de Assis, Patricia H. Suegama, Isolda G Costa, Michel Keddam, et al.. Influence of probe size for local electrochemical impedance measurements . *Electrochimica Acta*, 2017, 233, pp.256-261. 10.1016/j.electacta.2017.03.017 . hal-01492720

**HAL Id: hal-01492720**

<https://hal.sorbonne-universite.fr/hal-01492720v1>

Submitted on 20 Mar 2017

**HAL** is a multi-disciplinary open access archive for the deposit and dissemination of scientific research documents, whether they are published or not. The documents may come from teaching and research institutions in France or abroad, or from public or private research centers.

L'archive ouverte pluridisciplinaire **HAL**, est destinée au dépôt et à la diffusion de documents scientifiques de niveau recherche, publiés ou non, émanant des établissements d'enseignement et de recherche français ou étrangers, des laboratoires publics ou privés.

# Influence of probe size for local electrochemical impedance measurements

Caio Palumbo de Abreu,<sup>1,2</sup> Camila Molena de Assis,<sup>1,3</sup> Patricia Suegama,<sup>4</sup> Isolda Costa,<sup>2</sup> Michel Keddam,<sup>1</sup> Hercilio G. de Melo,<sup>3</sup> Vincent Vivier<sup>1,\*</sup>

<sup>1</sup>- Sorbonne Universités, UPMC Univ Paris 06, CNRS, Laboratoire Interfaces et Systèmes Electrochimiques, 4 place Jussieu, F-75005, Paris, France

<sup>2</sup>- Instituto de Pesquisas Energéticas e Nucleares, IPEN/CNEN-SP, Av. Prof. Lineu Prestes, 2242, CEP 05508-000, São Paulo, SP, Brazil

<sup>3</sup>- Departamento de Engenharia Metalúrgica e de Materiais, Escola Politécnica, Universidade de São Paulo, CP 61548, Zip Code 05424-970, São Paulo, SP, Brazil.

<sup>4</sup>- Faculdade de Ciências Exatas e Tecnologia – UFGD, Rodovia Dourados – Itahum, km 12, CP 364, Zip Code 79.804-970, Dourados, MS, Brazil

## Abstract

Local electrochemical impedance spectroscopy (LEIS) is a promising technique for the characterization of heterogeneous surface reactivity. Significant development of LEIS relies on the improvement of the spatial resolution for reaching the micrometer scale. This work presents a detailed analysis of the influence of the probe size, especially in the high frequency domain where an inductive-like response ascribed to the stray dielectric capacitance between the two electrodes of the probe used for performing the local current measurement can be observed. A detailed analysis of the whole set-up (electrode geometry and measuring device) allows an analytical expression of the impedance for the whole system to be obtained. Based on the analysis of this expression and on experimental results, two different strategies have been proposed to cancel the HF time constant: a post treatment of the results via a preliminary electrical characterization of the local probe or the minimization of the electrolyte resistance by

1 measuring the local potential in the close vicinity of the substrate. Both approaches were shown  
2 to be efficient.

3

4 *Keywords:* Local electrochemical impedance spectroscopy; local current density;  
5 microelectrodes; probe size; stray capacitance

6

7

## 1 **1. Introduction**


2 The characterization of the local reactivity of an electrified interface is usually performed with  
3 the use of local probes with an adequate size depending on the spatial resolution required, but  
4 also on the technique used. The scanning electrochemical microscopy (SECM) is by far the  
5 most widely used local technique in electrochemistry [1-3], but only few works have been  
6 performed in the frequency domain. For instance, the use of a single frequency measurements  
7 at an ultra-microelectrode (UME) allows to map the surface heterogeneity [4-7], whereas the  
8 use of the ac-SECM in substrate generation – tip collection mode allows a complex collection  
9 efficiency to be obtained, and thus to study the formation and the relaxation of reaction  
10 intermediates involved in complex mechanisms such as the proton reduction [8, 9] or the iron  
11 oxidation [10]. On the other hand, local current-density can be measured using the scanning  
12 vibrating electrode technique (SVET) [11-13] without the requirement of adding any redox  
13 mediator in solution. This technique then gives rise to the local electrochemical impedance  
14 spectroscopy (LEIS) as an alternative route for the local investigation of an electrochemical  
15 reaction, which has been developed in the 90's with the pioneering works of Isaacs *et al.* [14,  
16 15]. It consists in using two reference electrodes (*e.g.* a bi-microelectrode) that are positioned  
17 close to the interface of interest for measuring the local current density in solution from the  
18 potential difference between the two micro-reference electrodes immersed in the electrolyte.  
19 The current is thus measured as the ohmic drop between the two sensing electrodes in solution,  
20 and depends on both the electrode distance and the electrolyte conductivity. Thus, the local  
21 impedance can be calculated similarly to a usual (*i.e.* global) electrochemical impedance using  
22 a frequency response analyzer, that is as the ratio of the potential to the local current density  
23 for each frequency [14]. This technique was successfully used for the investigation of coating  
24 degradation [16-18], pitting corrosion of iron chromium alloy [19, 20], magnesium alloy  
25 corrosion [21], or time-constant distribution of a passive film formed on a stainless steel sample

1 [22]. However, one of the key-points for the technique is the spatial resolution that is governed  
2 by the probe size and the probe-to-sample distance. Indeed, for many applications such as  
3 coating degradation [16, 18], a spatial resolution in the millimeter range is usually sufficient,  
4 but for other applications such as the mapping of surface reactivity that depends on the grain  
5 size [21] or for the characterization of a single pit [19], a spatial resolution of few tens of  
6 micrometers is required. This can be obtained by diminishing both the size of each wire used  
7 for sensing the local potential in solution and the distance between these two wires. In this  
8 work, a specific attention has been paid to the response of local probes of few ten micrometers,  
9 since in the high frequency domain, a capacitive coupling may exist between two adjacent  
10 micro-wires, whereas in the low frequency domain, the potential difference to be measured  
11 between these two probes can be very small. A detailed analysis of experimental results was  
12 thus provided for a model system involving redox mediators studied at a metallic electrode,  
13 thus allowing the separation of the electrochemical contribution from the stray contribution of  
14 the measurement setup.

## 15 **2. Experimental**

16 All the electrochemical measurements were performed using a home-made setup previously  
17 described [21, 23] and presented in Fig. 1. It consisted in a potentiostat with which the global  
18 impedance was measured allowing the surface averaged value of the electrode response to be  
19 recorded, whereas simultaneously, the local potential and the local current density were probed  
20 in solution with a bi-microelectrode [14, 24, 25]. Data acquisitions were performed using a 4-  
21 channel frequency response analyzer (1254 – Solartron) allowing multiple transfer functions to  
22 be measured simultaneously. The probe positioning was achieved with stepper motors  
23 (UTM25, Newport) driven by a motion encoder (MM4005, Newport) allowing a spatial  
24 resolution of 0.2  $\mu\text{m}$  in the three directions. A homemade DC-offset coupled with a variable  
25 gain differential amplifier was used for the measurement of the local potential difference in

1 solution (*vide infra*). With such a configuration, it was possible to measure a potential  
 2 difference of *ca* 1  $\mu\text{V}$  between the two probes in the low frequency domain ( $f < 100$  mHz).  
 3 Interestingly, this limit can be lowered by adapting the amplification stages before and after the  
 4 DC-offset as a function of the local impedance to be measured. The distance between the probe  
 5 and the substrate was controlled by slowly bringing the probe in contact with the substrate and  
 6 then by withdrawing it to the desired distance. This allowed a vertical positioning with a  
 7 resolution of  $\pm 5$   $\mu\text{m}$ , which was estimated with an independent set of experiments.

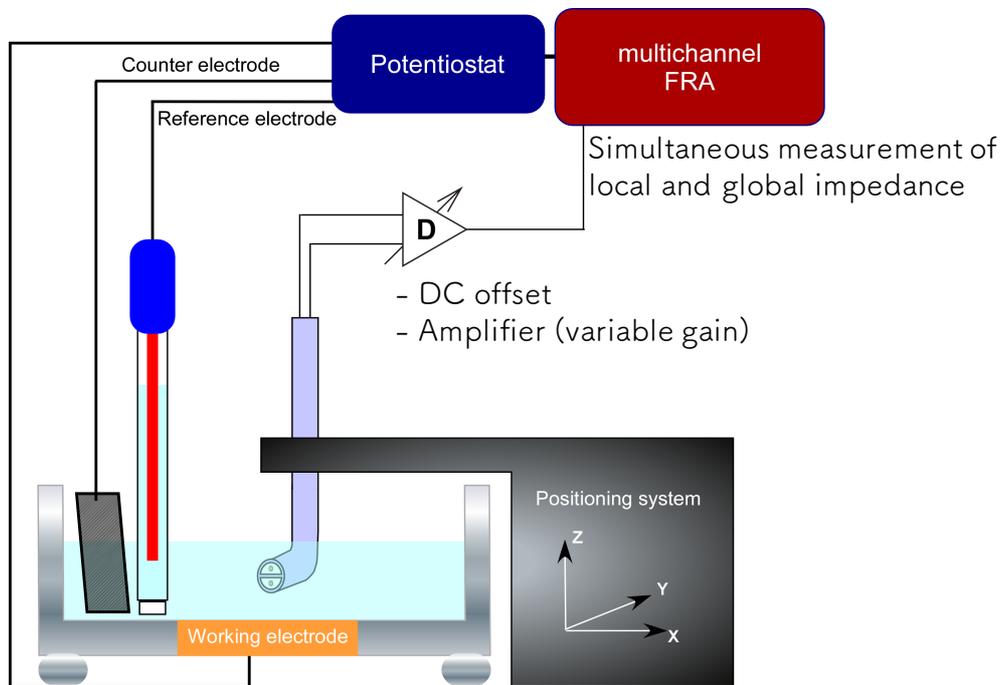

8  
 9 *Figure 1: Sketch of the experimental setup*

10 The working electrode was a platinum rod of 0.5 cm in diameter laterally insulated by a  
 11 cataphoretic paint (200 V / 2 minutes, then cured for 1 hour at 80°C) and an epoxy-resin  
 12 (Radiospare), thus exposing a disk of 0.2 cm<sup>2</sup> surface area to the electrolyte. No specific  
 13 activation of the electrode has been performed before the experiments. The counter electrode  
 14 was a platinum gauze of large surface area surrounding the whole electrochemical cell in order  
 15 to minimize the frequency dispersion due to the geometry of the system, and the reference  
 16 electrode was a saturated calomel electrode ( $E / \text{SCE} = E / \text{NHE} - 0.244$  V, where NHE is the

1 normal hydrogen electrode).


2 The local probe used for performing local impedance measurements consisted in a bi-  
3 microelectrode prepared with silver microwires laterally insulated with a cataphoretic paint  
4 (200 V / 1 minute, then cured for 1 hour at 80°C) and sealed with an epoxy-resin in a capillary.  
5 The apex of the probe was polished and each of the wires was anodized in a chloride containing  
6 solution to obtain an Ag/AgCl reference electrode. This procedure is in marked contrast to the  
7 use of platinum probes since it allows to minimize the contribution of the Nernst potential due  
8 to redox species in solution [26].

9 The spatial resolution that can be reached with such a probe depends on the size of the  
10 microwires, the distance between the two microwire centers ( $d$ ), and the distance between the  
11 probe and the substrate ( $h$ ) as sketched in Fig. 2. In addition, even if nanoelectrodes are  
12 available, the use of probe smaller than 1 mm is still challenging with respect to the potential  
13 measurement to be performed [27]. In this work, local impedance measurements were  
14 performed either by measuring the local current with the local probe and the global potential,  
15 or by measuring the local current with the local probe and the local potential with the closest  
16 probe to the electrode surface, similarly to the definition of Bayet *et al.* [28], emphasized later  
17 on by Huang *et al.* [27]. It is interesting to mention that the former experiment corresponds to  
18 the local impedance that can be usually measured with commercial equipment and will be  
19 labelled as local impedance in the following, whereas for the second definition, a home-made  
20 equipment is required and will be labelled local interfacial impedance [27].

21 Some electrical impedance measurements were performed with a dielectric interface (Solartron  
22 1296A) coupled to a frequency response analyzer (Solartron 1255) for the characterization of  
23 the probes.

1 All electrolytic solutions (10 mM ferri/ferrocyanide + 0.5 M KCl) were prepared with analytical  
2 grade chemicals in twice distilled water.

3

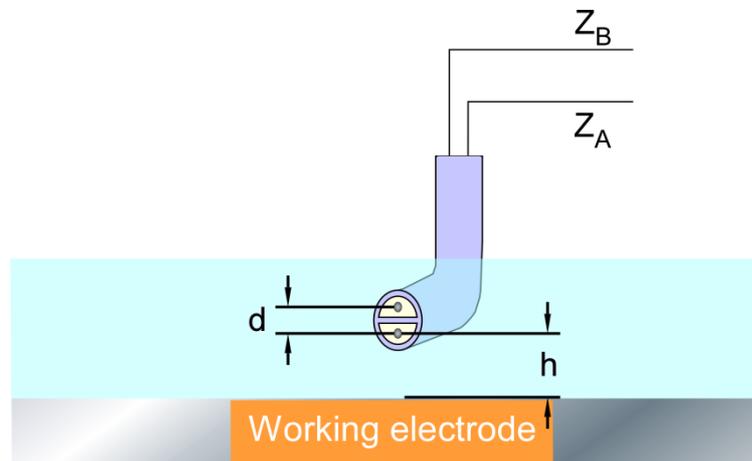

4

5 *Figure 2: Sketch of local probe with the relevant parameters investigated in this work*

### 6 **3. Results and discussion**


7 Figure 3a shows the global impedance diagram in a Nyquist representation obtained at a 5 mm  
8 in diameter platinum electrode for the ferri/ferrocyanide redox couple (10 mM) in 0.5 M KCl  
9 electrolytic solution. The EIS response is typical of a redox system in solution. It shows the  
10 electrolyte resistance as the high frequency limit, a capacitive loop ascribed to the charge  
11 transfer resistance in parallel with the double layer capacitance (with a characteristic frequency  
12 of about 900 Hz), and the Warburg impedance corresponding to the diffusion of the  
13 electroactive species. Interestingly, the local impedance response presented in Fig. 3b and  
14 measured above the Pt electrode center with a bi-electrode (each Ag/AgCl microelectrode was  
15 150  $\mu\text{m}$  in diameter and the distance between the two wires was 150  $\mu\text{m}$ ) shows the same  
16 behavior for the impedance response of the system, with the same time-constants and a similar  
17 amplitude. It should however be mentioned that the electrolyte resistance may be different from  
18 one experiment to the other, since, for local measurement, it depends not only on the electrolyte

1 conductivity, but also on the probe to substrate distance. In addition, Ferrari et al. showed that  
2 the global impedance response is not affected by the probe position above the electrode [29].  
3 Indeed, it was shown that whatever the probe position (close to the electrode center, or close to  
4 the electrode edge), that is, at locations where the local current densities are different, the global  
5 impedance response remains unchanged for both the amplitude of the different contributions  
6 and the time-constant. Therefore, any screening of the global current-potential distribution by  
7 the probe may be disregarded.

8 The low frequency limit is usually difficult to measure with a good accuracy. This is due to the  
9 fact that for most electrochemical systems, the magnitude of the low frequency impedance is  
10 larger than the high frequency contribution, in other words, the ac current to be measured  
11 decreases with the frequency. In the literature, this problem is often circumvented by decreasing  
12 the electrolyte concentration (*i.e.* by working in low conductive medium to optimize the  
13 resolution) [30]. However, such a choice strongly modifies the electrochemical system  
14 properties and results in difficulties for comparison with literature data. Indeed, the main  
15 drawback for the measurement is the dc-potential difference that exists between the two probes  
16 used to sense the local potential, which can however be corrected using a level shifter to  
17 improve the accuracy of the measurement, that is by adjusting the dc potential offset to 0 mV  
18 with a preliminary experiment performed in the same electrolyte [31]. It should also be  
19 mentioned that the use of a scanning vibrating electrode technique (SVET) provides another  
20 way to discard the residual dc-potential contribution that always exists between two different  
21 electrodes [28, 32]. Thus, the use of an intermediate low gain amplifier to initially correct the  
22 dc offset allows to work in concentrated electrolyte as it was done in this work (0.5 M KCl  
23 solution).

24 The same local experiment was performed with a smaller probe, namely, two Ag/AgCl  
25 microelectrodes of 20  $\mu\text{m}$  in diameter each, separated by a distance of about 15  $\mu\text{m}$  (Fig. 4).


1 The LEIS responses are similar with either a large or a small probe except in the high frequency  
 2 domain for which an inductive behavior is observed when the distance between the two  
 3 Ag/AgCl wires is decreased. This kind of response is usually encountered in the case of studies  
 4 on large batteries because of the stray impedance (*i.e.* inductance) of the wires used for  
 5 measuring the very low impedance systems, but this hypothesis must be ruled out in the case  
 6 of localized impedance since the measured quantities are in the ohm range or larger.

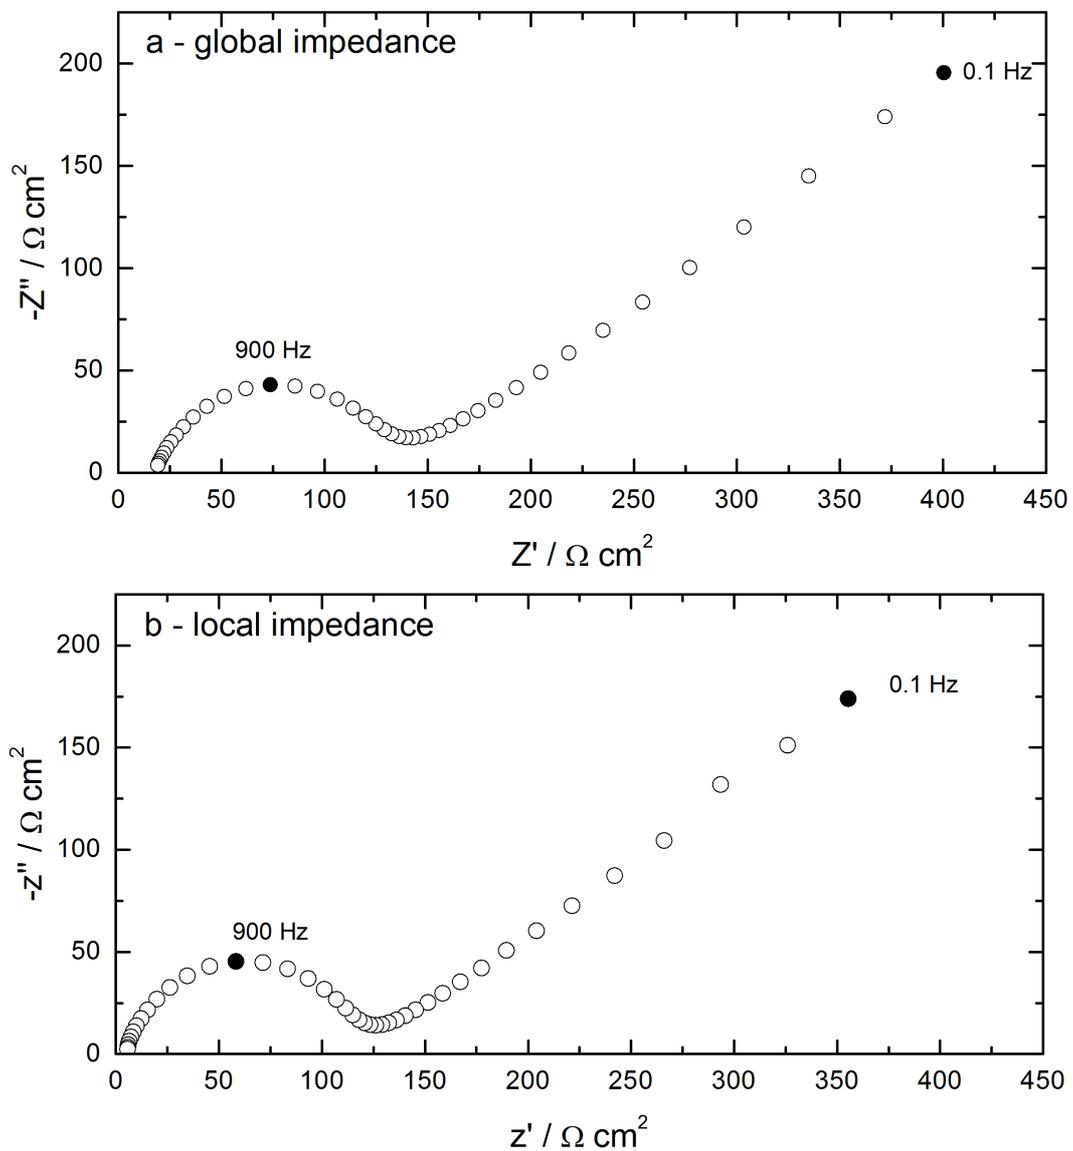

7

8 *Figure 3: EIS and LEIS diagrams recorded simultaneously in a ferri/ferrocyanide (10 mM) +*  
 9 *0.5 M KCl electrolyte at the equilibrium potential ( $E = 0.195 \text{ V/SCE}$ ). The distance between*  
 10 *the two wires and the radius of each wire were  $150 \mu\text{m}$ ; probe-to-sample distance  $h=100 \mu\text{m}$ .*

11

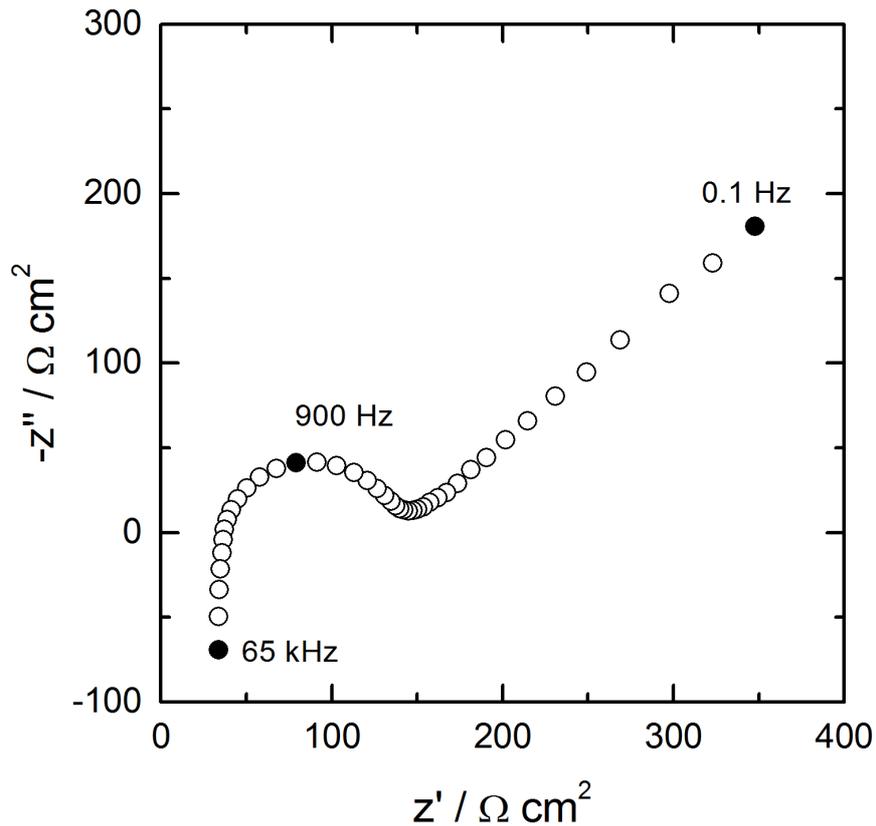


1

2 *Figure 4: LEIS diagrams measured with a small probe (diameter of each wire: 20 μm;*  
 3 *distance between wires: 15 μm; probe-to-sample distance h=100 μm) in a ferri/ferrocyanide*  
 4 *(10 mM) + 0.5 M KCl electrolytic solution at the equilibrium potential.*

5

6

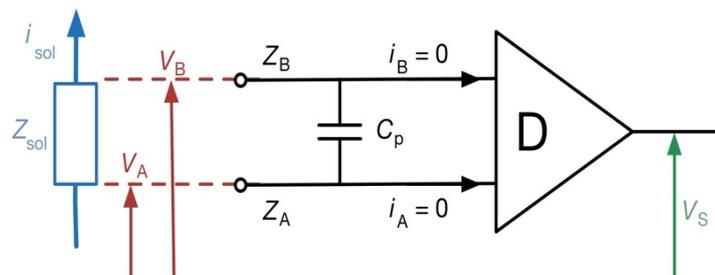

7

8 *Figure 5: Electrical circuit describing the local current amplification set-up from the*  
 9 *measurement of the local potential difference between two probes.*

10

11 In fact, this effect can be understood by modelling more precisely how the ac potential actually  
 12 measured between the two electrodes depends on their own electrochemical impedances, the  
 13 inter-electrode dielectric capacitance and the resistance of the potential source in solution. Let

1 us consider the electrical sketch of the setup used for performing the measurement (Fig. 5). It  
 2 consisted in a differential amplifier, the two inputs of which are connected to the Ag/AgCl  
 3 microreference electrodes. The short distance between the two wires gives rise to a stray  
 4 capacitance,  $C_p$ , whereas the impedance of each probe is  $Z_A$  and  $Z_B$ . The local potential  
 5 difference,  $\Delta V_{probe} = V_B - V_A$ , measured between the two probes allows the local current  
 6 density,  $j_{loc}$ , to be readily calculated as

$$7 \quad j_{loc} = \frac{\Delta V_{probe}}{\rho d} \quad Eq. 1$$

8 where  $\rho$  is the electrolyte conductivity and  $d$  the distance between the two probes. This quantity  
 9 corresponds to the actual local current density flowing in the solution and sensed by the  
 10 microprobe at a distance  $h$  of the interface. Assuming an ideal behavior of the differential  
 11 amplifier, that is infinite input impedance, infinite open-circuit gain and flat band-pass, only  
 12 the impedance of the individual microelectrodes and the stray capacitance have to be taken into  
 13 account as parasitic effects in the measurement of the local current density. The current,  $i_c$ ,  
 14 flowing in the capacitance can thus be expressed as


$$15 \quad i_c = \frac{j_{loc} \rho d}{Z_A + \frac{1}{j\omega C_p} + Z_B} \quad Eq. 2$$

16 and the potential difference,  $\Delta V_{diff}$ , between the two inputs of the differential amplifier is given  
 17 by

$$18 \quad \Delta V_{diff} = \frac{i_c}{j\omega C_p} = \frac{j_{loc} \rho d}{j\omega C_p(Z_A + Z_B) + 1} \quad Eq. 3$$

19 The stray capacitance can be independently determined by measuring the impedance of the  
 20 microreference electrodes in air, as shown in Fig. 6. A capacitive behavior was obtained with a  
 21 low frequency limit in the range of  $G\Omega$ , and a capacitance of about 7 pF from the fit of the  
 22 experimental results with a Voigt element. It should be mentioned that this value was not  
 23 obtained with a usual potentiostat but with a dielectric interface, which allows such a low value  
 24 to be measured.

1

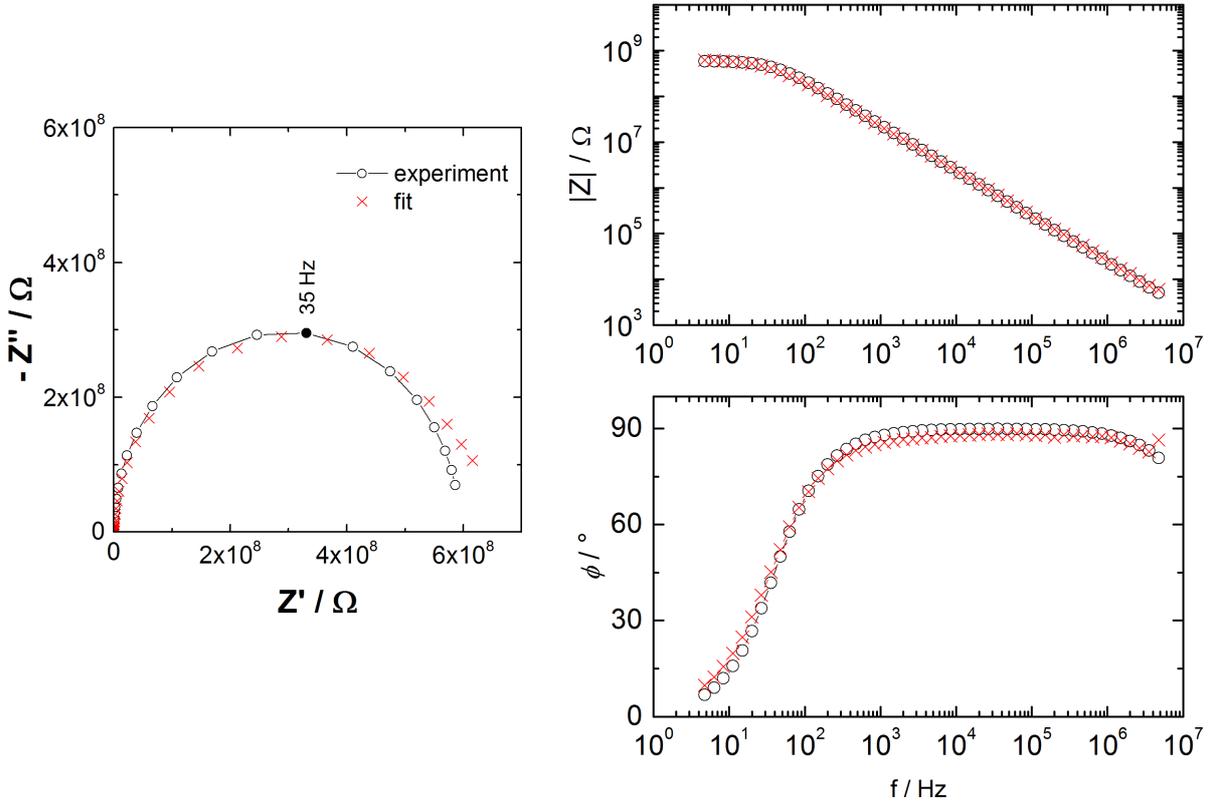

2

3 *Figure 6: Impedance diagram in Nyquist and Bode representation measured with a bi-*  
 4 *microelectrode in air (open circles) and result of the fitting (red crosses) with a RC time*  
 5 *constant (Voigt element) for the evaluation of the stray capacitance*

6

7 Moreover, the stray capacitance also depends on the distance between the two wires as usually

8 observed for the patterns of printed circuit boards measured in the high frequency range [33].

9 Additionally, when the experiment is performed in an electrolytic solution, similar impedance

10 diagrams were obtained but with a larger stray capacitance (between 25 to 100 pF), the value

11 of which depends on the electrolyte conductivity. This was ascribed to the additional capacitive

12 contribution introduced by the ac current path connecting the two microprobes through the

13 surrounding electrolyte.

14 Similarly, the impedance of each microelectrode was obtained by measuring independently

15 their electrochemical impedance in the electrolyte at the equilibrium potential, *i.e.* when no

1 current flow between the two electrodes (data not presented), which shows that the impedance  
 2 of each probe can be expressed as

$$3 \quad Z_A = R_1 + \frac{R_2}{1+j\omega R_2 C} \quad Eq. 4$$

4  $R_2$  and  $C$  (the capacitance of the electrode immersed in solution, that is the combination of the  
 5 double layer capacitance and that of the thin AgCl layer at the Ag microelectrode surface)  
 6 depend only on the probe geometry, whereas  $R_1$  depends on the distance between the two  
 7 microwires. As the two probes used for measuring the local current density are assumed to be  
 8 identical,  $Z_A = Z_B$  and Eq. 3 can be rewritten as

$$9 \quad \Delta V_{diff} = \frac{i_c}{j\omega C_p} = \frac{j_{loc} \rho d}{j\omega C_p 2 \left( R_1 + \frac{R_2}{1+j\omega R_2 C} \right) + 1} \quad Eq. 5$$

10 Thus, the local current density can be obtained from

$$11 \quad j_{loc} = \frac{\Delta V_{diff}}{\rho d} \left( j\omega C_p 2 \left( R_1 + \frac{R_2}{1+j\omega R_2 C} \right) + 1 \right) \quad Eq. 6$$

12 and the local impedance measured by the experimental setup,  $Z_{measured}$ , is expressed as

$$13 \quad Z_{measured} = \frac{\Delta V_{applied}}{j_{loc}} = \frac{\Delta V_{applied}}{\frac{\Delta V_{diff}}{\rho d} \left( j\omega C_p 2 \left( R_1 + \frac{R_2}{1+j\omega R_2 C} \right) + 1 \right)} \quad Eq. 7$$

14 where  $\Delta V_{applied}$  is the applied potential between the substrate and the reference electrode. Thus  
 15 the local impedance corresponding to the electrochemical contribution of the system corrected  
 16 from the stray effect is obtained from

$$17 \quad Z_{loc} = Z_{measured} \left( j\omega C_p 2 \left( R_1 + \frac{R_2}{1+j\omega R_2 C} \right) + 1 \right) \quad Eq. 8$$


18 Interestingly, in the low frequency domain ( $\omega \rightarrow 0$ ), the local impedance is not influenced by  
 19 the measuring device and

$$20 \quad \lim_{\omega \rightarrow 0} Z_{loc} = Z_{measured} \quad Eq. 9$$

1 whereas in the high frequency domain ( $\omega \rightarrow \infty$ ), where the inductive behavior was observed  
 2 for the local electrochemical impedance, the term  $\frac{R_2}{1+j\omega R_2 C}$  tends towards 0 and the local  
 3 impedance is thus expressed as

$$4 \quad z_{loc} = z_{measured} (2j\omega R_1 C_p + 1) \quad Eq. 10$$


5 This relation shows that the product  $R_1 C_p$  is involved in the equation, meaning that without any  
 6 independent determination of  $R_1$  or  $C_p$ , one can only get the product of these two quantities  
 7 from the fitting.

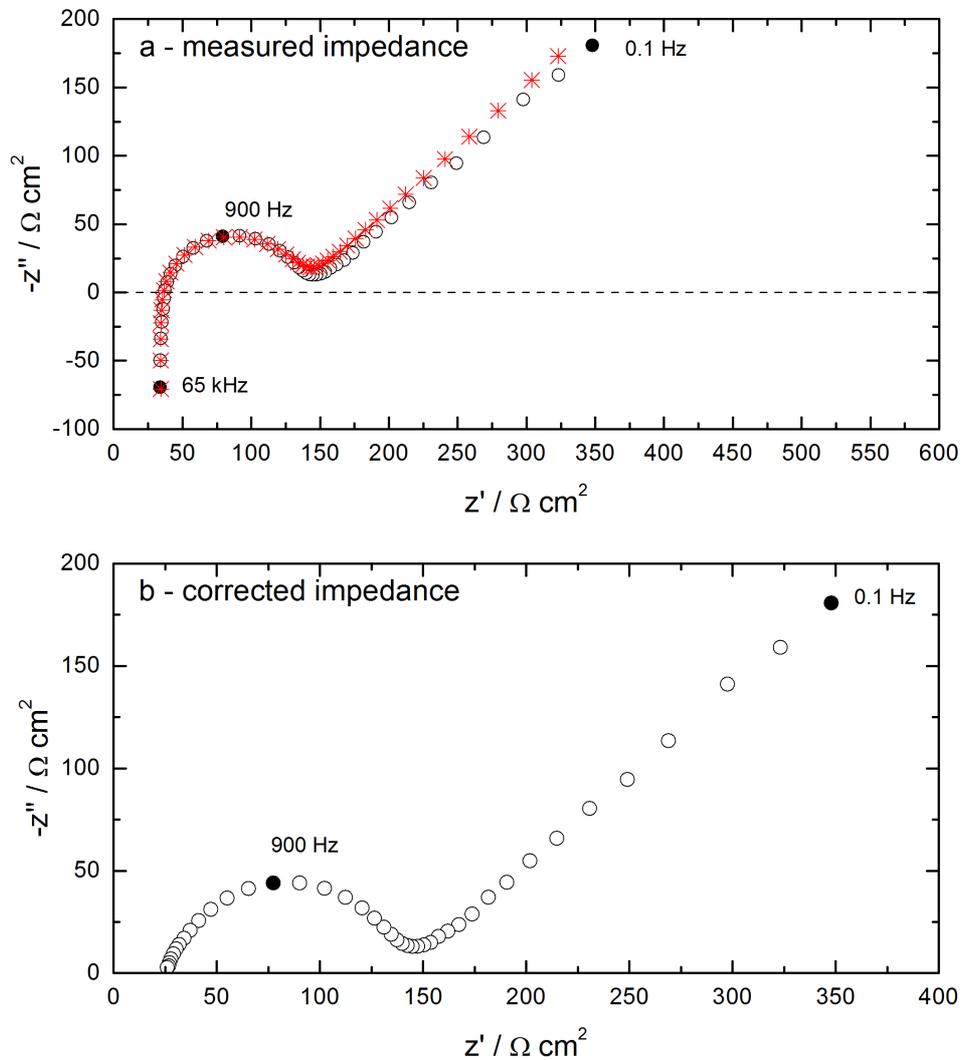

8

9 *Figure 7: Fit of the local impedance data using the Eq. 10 (a) and local impedance response*  
 10 *corrected from the stray capacitance (b). Diameter of each wire: 20  $\mu\text{m}$ ; distance between*  
 11 *wires: 15  $\mu\text{m}$ ; probe-to-sample distance  $h=100 \mu\text{m}$ .*

1 Fig. 7a shows the result of the local impedance fitting using Eq. 10 in combination with the  
 2 Randles equivalent circuit for describing the electron exchange reaction in solution. A very  
 3 good agreement with the experimental results is obtained. Moreover, the use of Eq. 10 allows  
 4 correcting the impedance diagrams from the high frequency contribution, as shown in Fig. 7b.  
 5 This local impedance diagram is very similar to the experimental result presented in Fig. 3 with  
 6 a larger probe size, showing that it is possible to decrease the probe size, and thus to increase  
 7 the spatial resolution for the LEIS measurement. Interestingly, a careful analysis of Eq. 10  
 8 shows that the corrective term that accounts for the stray capacitance multiplies the actual local  
 9 impedance. In the high frequency domain, the local impedance response is dominated by the  
 10 electrolyte resistance, thus the effect of the stray capacitance can be minimized by decreasing  
 11 the electrolyte resistance, that is, by increasing the electrolyte conductivity or by decreasing the  
 12 probe to sample distance.

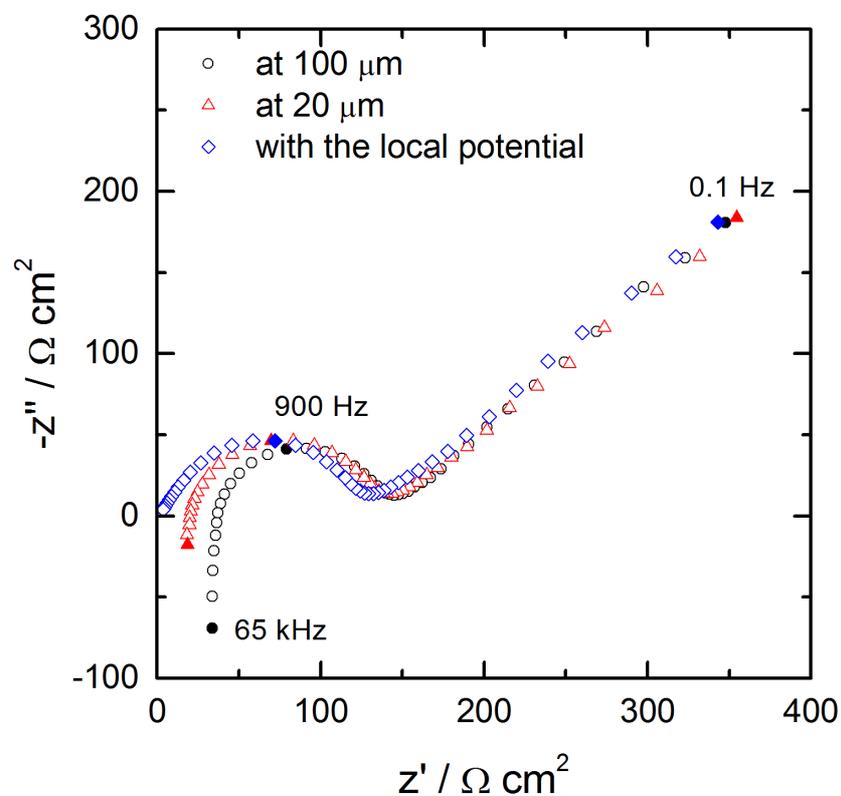

13

14 *Figure 8: Influence of the probe position on the HF behavior of the local impedance (black*  
 15 *circles and red triangles) and the local interfacial impedance (blue diamonds). Diameter of*  
 16 *each wire: 20 μm; distance between wires: 15 μm.*

1 Figure 8 shows the influence of the probe-to-sample distance on the local impedance response,  
2 using the same probe. A significant effect can be seen in the high frequency behavior (black  
3 and red symbols). First, a shift towards higher electrolyte resistance value is observed as the  
4 distance increases, which is accompanied by an increase of the  $R_1C_p$  time-constant in this  
5 frequency domain. This is due to the fact that the uncompensated ohmic drop contribution  
6 increases with the distance. In order to decrease this contribution, a possible solution is to  
7 measure both the local potential, and the local current density for the evaluation of the local  
8 interfacial impedance as previously performed in the literature for measuring the local  
9 interfacial impedance [27, 32]. In that case, the contribution of the electrolyte resistance is  
10 vanishingly small consistently with the short electrolyte path between the probe and the surface  
11 as shown in Fig. 8 (blue curve) and the local interfacial impedance result remains free from the  
12 stray capacitance contribution, even when the measurement was performed with a small probe.  
13 It should also be mentioned that the contribution of the electrolyte resistance is likely to depend  
14 on the particular location of the probe both in distance from the surface and along a radius of  
15 the electrode since it is determined by the local electrolyte resistivity and the current-potential  
16 field in the solution.

17

#### 18 **4. Conclusions**

19 The local impedance spectroscopy can be performed using different probe sizes. When a small  
20 probe is used, *i.e.* in the range of few tens of micrometers or less, the high frequency domain  
21 shows an inductive behavior that was ascribed to the presence of a stray capacitance between  
22 the two wires forming the probe. It was also shown that LEIS diagrams can be easily corrected  
23 by a numerical post-treatment in as much as a preliminary characterization of the probe was  
24 made. From the modeling of the measuring device, it was shown that the time constant due to  
25 the combination of the stray capacitance and the electrolyte resistance is in the measurable

1 domain, and the electrolyte resistance must be decreased in order to minimize the high-  
2 frequency contribution, in agreement with experimental results performed for different probe  
3 positions above the substrate. Moreover, this effect can also be minimized by measuring the  
4 local potential instead of the global one, that is, the local interfacial impedance. In that case, the  
5 ohmic contribution is governed by the distance between the closest wire of the probe used for  
6 measuring the local current density and the substrate. The spatial resolution of the LEIS  
7 technique can thus be improved for reaching the micrometer scale using the local interfacial  
8 impedance to avoid the high frequency inductive behavior.

## 9 **5. Acknowledgements**

10 CAPES (BEX 7307/14-4) and COFECUB (Project N° 806-14) are gratefully acknowledged for  
11 their financial support.

## Bibliography

- 1  
2
- 3 [1] G. Wittstock, Imaging localized reactivities of surfaces by scanning electrochemical  
4 microscopy, *Topics in Applied Physics*, 85 (2003) 335-364.
- 5 [2] M.V. Mirkin, W. Nogala, J. Velmurugan, Y. Wang, Scanning electrochemical microscopy  
6 in the 21st century. Update 1: five years after, *Phys. Chem. Chem. Phys.*, 13 (2011) 21196-  
7 21212.
- 8 [3] D. Polcari, P. Dauphin-Ducharme, J. Mauzeroll, Scanning Electrochemical Microscopy: A  
9 Comprehensive Review of Experimental Parameters from 1989 to 2015, *Chemical Reviews*,  
10 116 (2016) 13234-13278.
- 11 [4] K. Eckhard, W. Schuhmann, Alternating current techniques in scanning electrochemical  
12 microscopy (AC-SECM), *Analyst*, 133 (2008) 1486-1497.
- 13 [5] A.S. Bandarenka, K. Eckhard, A. Maljusch, W. Schuhmann, Localized electrochemical  
14 impedance spectroscopy: visualization of spatial distributions of the key parameters  
15 describing solid/liquid interfaces, *Anal Chem*, 85 (2013) 2443-2448.
- 16 [6] C. Gabrielli, F. Huet, M. Keddam, P. Rousseau, V. Vivier, Scanning Electrochemical  
17 Microscopy Imaging by Means of High-Frequency Impedance Measurements in Feedback  
18 Mode, *J. Phys. Chem. B*, 108 (2004) 11620-11626.
- 19 [7] C. Gabrielli, E. Ostermann, H. Perrot, V. Vivier, L. Beitone, C. Mace, Concentration  
20 mapping around copper microelectrodes studied by scanning electrochemical microscopy,  
21 *Electrochem. Commun.*, 7 (2005) 962-968.
- 22 [8] D. Trinh, M. Keddam, X.R. Nova, V. Vivier, Alternating-Current Measurements in  
23 Scanning Electrochemical Microscopy, Part 1: Principle and Theory, *ChemPhysChem*, 12  
24 (2011) 2169-2176.
- 25 [9] D. Trinh, M. Keddam, X.R. Nova, V. Vivier, Alternating Current Measurements in  
26 Scanning Electrochemical Microscopy, Part 2: Detection of Adsorbates, *ChemPhysChem*, 12  
27 (2011) 2177-2183.
- 28 [10] D. Trinh, M. Keddam, X.R. Nova, V. Vivier, Characterization of adsorbates by  
29 transient measurements in Scanning Electrochemical Microscopy, *Electrochim. Acta*, 131  
30 (2014) 28-35.
- 31 [11] L.F. Jaffe, R. Nuccitelli, An ultrasensitive vibrating probe for measuring steady  
32 extracellular currents, *J Cell Biol*, 63 (1974) 614-628.
- 33 [12] H.S. Isaacs, The measurement of the galvanic corrosion of soldered copper using the  
34 scanning vibrating electrode technique, *Corros. Sci.*, 28 (1988) 547-558.
- 35 [13] H.S. Isaacs, Initiation of stress corrosion cracking of sensitized type 304 stainless steel in  
36 dilute thiosulfate solution, *J. Electrochem. Soc.*, 135 (1988) 2180-2183.
- 37 [14] R.S. Lillard, P.J. Moran, H.S. Isaacs, A novel method for generating quantitative local  
38 electrochemical impedance spectroscopy, *J. Electrochem. Soc.*, 139 (1992) 1007-1012.

- 1 [15] F. Zou, D. Thierry, H.S. Isaacs, A high-resolution probe for localized electrochemical  
2 impedance spectroscopy measurements, *J. Electrochem. Soc.*, 144 (1997) 1957-1965.
- 3 [16] V. Upadhyay, D. Battocchi, Localized electrochemical characterization of organic  
4 coatings: A brief review, *Progress in Organic Coatings*, 99 (2016) 365-377.
- 5 [17] J.V. Nardeli, D.V. Snihirova, C.S. Fugivara, M.F. Montemor, E.R.P. Pinto, Y.  
6 Messaddecq, A.V. Benedetti, Localised corrosion assesement of crambe-oil-based  
7 polyurethane coatings applied on the ASTM 1200 aluminum alloy, *Corros. Sci.*, 111 (2016)  
8 422-435.
- 9 [18] E. Aragon, C. Merlatti, J.B. Jorcin, N. Pebere, Study of delamination of organic coatings  
10 by local electrochemical impedance spectroscopy, *Eur.Fed.Corros.Publ.*, 45 (2007) 62-70.
- 11 [19] I. Annergren, D. Thierry, F. Zou, Localized electrochemical impedance spectroscopy for  
12 studying pitting corrosion on stainless steels, *J. Electrochem. Soc.*, 144 (1997) 1208-1215.
- 13 [20] I. Annergren, F. Zou, D. Thierry, Application of localized electrochemical techniques to  
14 study kinetics of initiation and propagation during pit growth, *Electrochim. Acta*, 44 (1999)  
15 4383-4393.
- 16 [21] G. Galicia, N. Pebere, B. Tribollet, V. Vivier, Local and global electrochemical  
17 impedances applied to the corrosion behaviour of an AZ91 magnesium alloy, *Corros. Sci.*, 51  
18 (2009) 1789-1794.
- 19 [22] I. Frateur, V.M. Huang, M.E. Orazem, B. Tribollet, V. Vivier, Experimental Issues  
20 Associated with Measurement of Local Electrochemical Impedance, *J. Electrochem. Soc.*,  
21 154 (2007) C719-C727.
- 22 [23] I. Frateur, V.M.-W. Huang, M.E. Orazem, N. Pebere, B. Tribollet, V. Vivier, Local  
23 electrochemical impedance spectroscopy: Considerations about the cell geometry,  
24 *Electrochim. Acta*, 53 (2008) 7386-7395.
- 25 [24] V.M.-W. Huang, V. Vivier, I. Frateur, M.E. Orazem, B. Tribollet, The global and local  
26 impedance response of a blocking disk electrode with local constant-phase-element behavior,  
27 *J. Electrochem. Soc.*, 154 (2007) C89-C98.
- 28 [25] J.B. Jorcin, E. Aragon, C. Merlatti, N. Pebere, Delaminated areas beneath organic  
29 coating: A local electrochemical impedance approach, *Corros. Sci.*, 48 (2006) 1779-1790.
- 30 [26] I. Frateur, E. Bayet, M. Keddam, B. Tribollet, Local redox potential measurement,  
31 *Electrochem. Commun.*, 1 (1999) 336-340.
- 32 [27] V.M.-W. Huang, S.-L. Wu, M.E. Orazem, N. Pebere, B. Tribollet, V. Vivier, Local  
33 electrochemical impedance spectroscopy: A review and some recent developments,  
34 *Electrochim. Acta*, 56 (2011) 8048-8057.
- 35 [28] E. Bayet, F. Huet, M. Keddam, K. Ogle, H. Takenouti, A novel way of measuring local  
36 electrochemical impedance using a single vibrating probe, *J. Electrochem. Soc.*, 144 (1997)  
37 L87-L90.

- 1 [29] J.V. Ferrari, M.H.G. De, M. Keddam, M.E. Orazem, N. Pebere, B. Tribollet, V. Vivier,  
2 Influence of normal and radial contributions of local current density on local electrochemical  
3 impedance spectroscopy, *Electrochim. Acta*, 60 (2012) 244-252.
- 4 [30] G. Baril, C. Blanc, M. Keddam, N. Pebere, Local electrochemical impedance  
5 spectroscopy applied to the corrosion behavior of an AZ91 magnesium alloy, *J. Electrochem.*  
6 *Soc.*, 150 (2003) B488-B493.
- 7 [31] N. Pébère, V. Vivier, Local Electrochemical Measurements in Bipolar Experiments for  
8 Corrosion Studies, *ChemElectroChem*, 3 (2016) 415-421.
- 9 [32] E. Bayet, F. Huet, M. Keddam, K. Ogle, H. Takenouti, Local electrochemical impedance  
10 measurement: scanning vibrating electrode technique in ac mode, *Electrochim. Acta*, 44  
11 (1999) 4117-4127.
- 12 [33] R. Sihlbom, M. Dernevik, M. Lindgren, J.P. Starski, Z. Lai, J. Liu, High frequency  
13 measurements and simulations on wire-bonded modules on the sequential build-up boards  
14 (SBU's), *IEEE Transactions on Components Packaging and Manufacturing Technology Part*  
15 *A*, 21 (1998) 478-491.
- 16