



HAL
open science

Low Temperature NMR Study of Silicophosphate Materials

Cristina Coelho, Guillaume Laurent, Christian Bonhomme

► **To cite this version:**

Cristina Coelho, Guillaume Laurent, Christian Bonhomme. Low Temperature NMR Study of Silicophosphate Materials. 9ème réunion de travail RMN du solide d'Eveux, Nov 2006, La Baume, France. hal-01881898

HAL Id: hal-01881898

<https://hal.sorbonne-universite.fr/hal-01881898v1>

Submitted on 26 Sep 2018

HAL is a multi-disciplinary open access archive for the deposit and dissemination of scientific research documents, whether they are published or not. The documents may come from teaching and research institutions in France or abroad, or from public or private research centers.

L'archive ouverte pluridisciplinaire **HAL**, est destinée au dépôt et à la diffusion de documents scientifiques de niveau recherche, publiés ou non, émanant des établissements d'enseignement et de recherche français ou étrangers, des laboratoires publics ou privés.

Low Temperature NMR Study of Silicophosphate Materials





C. COELHO, G. LAURENT, C. BONHOMME



Laboratoire de Chimie de la Matière Condensée de Paris, CNRS-Université Pierre et Marie Curie, Paris

Silicophosphate can be used as bioactive materials for the growing of hydroxyapatite, or for protonic conduction. They are also interesting models for the study of diatoms, organisms containing a biological part with phosphorous and a shell of silica. The aim of this work is to develop methods to study by NMR interactions between ^{31}P and ^{29}Si nuclei. Due to the mobility, it is difficult to see interactions at ambient temperature. In order to improve the signal to noise ratio and to study dynamic properties, we have used low temperature NMR. However, such study needs a special equipment and a rigorous calibration, which has been done using ^{207}Pb NMR on $\text{Pb}(\text{NO}_3)_2$ ¹. This nucleus is particularly sensitive to the temperature.

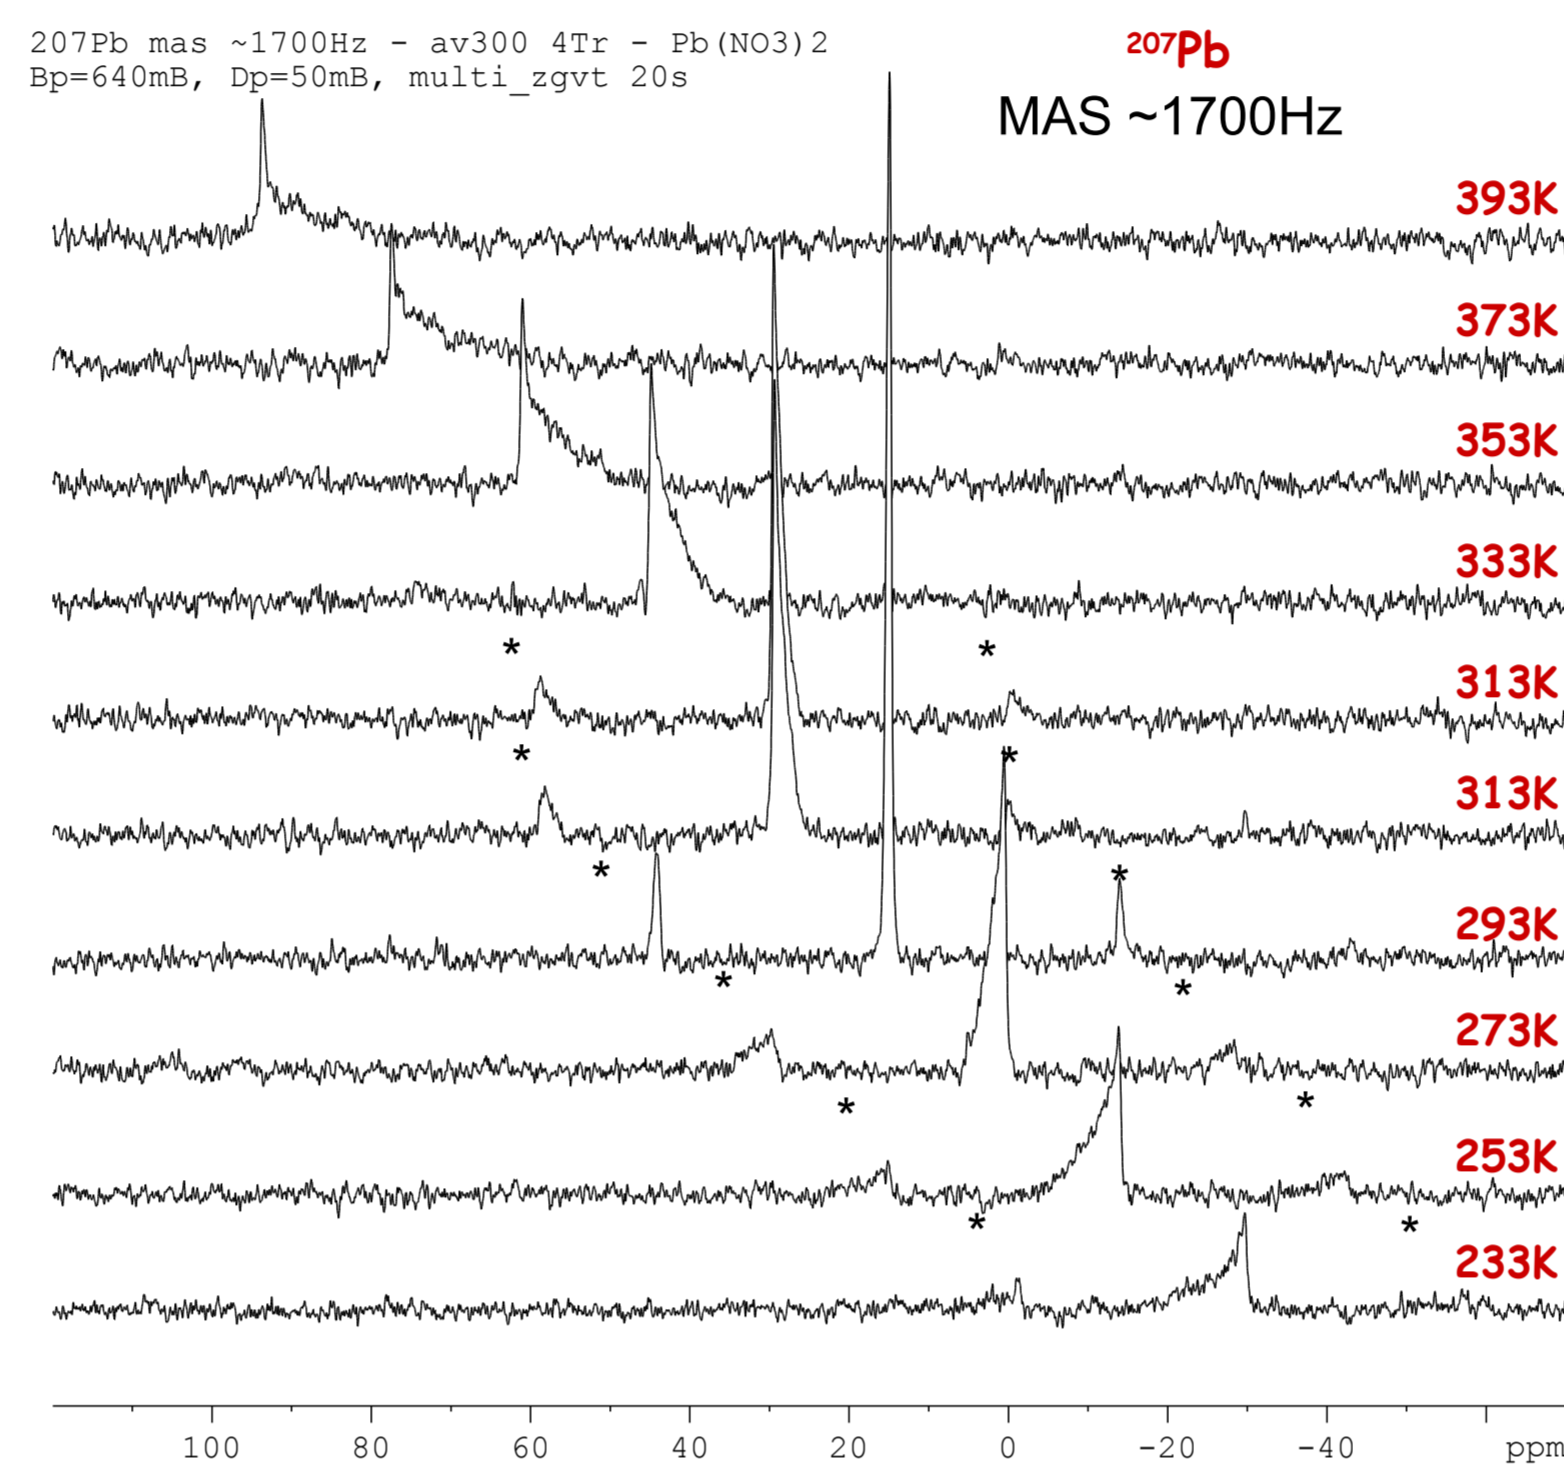

¹ Temperature Dependence of ^{207}Pb MAS spectra of Solid Lead Nitrate. An accurate, Sensitive Thermometer for Variable Temperature MAS, A. Bielecki and D. P. Burum, *J. Magn. Reson., Ser. A*, 116, 215-220 (1995).

