



**HAL**  
open science

# Routine monitoring of isometric knee extension strength in patients with muscle impairments using a new portable device: cross-validation against a standard isokinetic dynamometer

Jean-Yves Hogrel, Olivier Benveniste, Damien Bachasson

## ► To cite this version:

Jean-Yves Hogrel, Olivier Benveniste, Damien Bachasson. Routine monitoring of isometric knee extension strength in patients with muscle impairments using a new portable device: cross-validation against a standard isokinetic dynamometer. *Physiological Measurement*, 2020, 41 (1), pp.015003. 10.1088/1361-6579/ab6b49 . hal-02530660

**HAL Id: hal-02530660**

<https://hal.sorbonne-universite.fr/hal-02530660v1>

Submitted on 3 Apr 2020

**HAL** is a multi-disciplinary open access archive for the deposit and dissemination of scientific research documents, whether they are published or not. The documents may come from teaching and research institutions in France or abroad, or from public or private research centers.

L'archive ouverte pluridisciplinaire **HAL**, est destinée au dépôt et à la diffusion de documents scientifiques de niveau recherche, publiés ou non, émanant des établissements d'enseignement et de recherche français ou étrangers, des laboratoires publics ou privés.

1  
2  
3 1 Routine monitoring of isometric knee extension strength in patients with muscle  
4  
5  
6 2 impairments using a new portable device: cross-validation against a standard  
7  
8  
9 3 isokinetic dynamometer

10  
11 4  
12  
13 5 Jean-Yves Hogrel<sup>1</sup>, Olivier Benveniste<sup>2</sup>, Damien Bachasson<sup>1</sup>

14  
15  
16 6 <sup>1</sup>Institute of Myology, Neuromuscular Investigation Center, Pitié-Salpêtrière University  
17  
18 7 Hospital, Paris, France

19  
20 8 <sup>2</sup>Department of Internal Medicine and Clinical Immunology and Inflammation-  
21  
22 9 Immunopathology-Biotherapy Department (I2B), Pitié-Salpêtrière University Hospital,  
23  
24 10 Assistance Publique-Hôpitaux de Paris, East Paris Neuromuscular Diseases Reference Center,  
25  
26 11 Inserm U974, Sorbonne Université, Paris 6, Paris, France

27  
28  
29  
30 12

31  
32 13 **Corresponding author**

33  
34 14 Jean-Yves Hogrel

35  
36 15 Institut de Myologie

37  
38 16 Hôpital Universitaire Pitié-Salpêtrière

39  
40 17 75651 Paris Cedex 13

41  
42 18 France

43  
44 19 Phone: +33 1 42 16 58 80

45  
46 20 Fax: +33 1 42 16 58 81

47  
48 21 E-mail: [jy.hogrel@institut-myologie.org](mailto:jy.hogrel@institut-myologie.org)

49  
50  
51  
52 22  
53  
54  
55  
56  
57  
58  
59  
60

1  
2  
3 **Abstract**  
4

5 *Objective:* Muscle strength is a critical clinical hallmark in both health and disease. The  
6  
7  
8 current study introduces a novel portable device prototype (MyoQuad) for assessing and  
9  
10  
11  
12 monitoring maximal voluntary isometric knee extension torque (MVIT). *Approach:* Fifty-six  
13  
14  
15 patients with inclusion body myositis were studied. Knee extension weakness is a key feature  
16  
17  
18 in this inflammatory muscle disease. Cross-validation with an isokinetic dynamometer  
19  
20  
21 (Biodex System 3 Pro) was performed. Between-day reproducibility and ability to monitor  
22  
23  
24 changes in muscle strength over time compared to the gold standard method as a reference,  
25  
26  
27 were also investigated. *Main results:* The measurement was feasible even in the weakest  
28  
29  
30 patients. Agreement between methods was excellent (standard error of measurement (SEM)  
31  
32  
33 was 3.8 Nm and intra-class correlation coefficient (ICC) was 0.973). Least significant  
34  
35  
36 difference (LSD) was 4.9 and 5.3 Nm for the MyoQuad and the Biodex, respectively  
37  
38  
39 Measurements using the MyoQuad exhibited excellent between-day reproducibility (SEM  
40  
41  
42 was 2.4 Nm and ICC was 0.989 versus 2.6 Nm and 0.988 using the Biodex). Changes in  
43  
44  
45 MVIT at 6 and 12 months were similar between methods (timepoint  $\times$  method interaction was  
46  
47  
48 not significant; all  $p > 0.19$ ); strength changes classified according to LSD at 6 and 12 months  
49  
50  
51 were consistent between methods ( $>70\%$  consistent classification)). *Significance:* The  
52  
53  
54 measurement of maximal voluntary isometric knee extension torque using the MyoQuad  
55  
56  
57 offers a cost-effective, portable and immediate alternative for the routine measurement of  
58  
59  
60 maximal voluntary isometric strength of the quadriceps. The MyoQuad offers a comfort and  
stability that cannot be provided by standard hand-held dynamometers. These results support  
quantitative muscle strength assessment using fixed yet flexible dynamometry within clinical  
routine and multicenter trials.

1  
2  
3 47 **Keywords:** device; muscle strength dynamometer; muscle weakness; myositis; outcome

4  
5 48 measures

6  
7 49

8  
9  
10 50 **List of abbreviations**

11  
12 51 MMT, manual muscle testing; HHD, hand-held dynamometry; MVIT, maximal isometric

13  
14 52 knee extension voluntary torque; SD, standard deviation; CIM, change in mean; ICC, intra-

15  
16 53 class correlation coefficient; SEM, standard error of measurement; LSD, least significant

17  
18  
19 54 change

20  
21 55

## 56 **Introduction**

57 Muscle weakness has been demonstrated to be an independent predictor of all-cause mortality  
58 in an apparently healthy population ([Garcia-Hermoso et al., 2018](#)). Knee extension has been  
59 identified as a preferential target for detecting muscle weakness in various chronic disorders  
60 and other conditions such as aging or immobilization. Availability of a simple portable setup  
61 and methodology for assessing knee extensor strength is critical to generalize the  
62 measurement of this important clinical hallmark.

63 Strength assessment within clinical settings is most frequently performed using manual  
64 muscle testing (MMT) ([Hogrel et al., 2006](#)). As a semi-quantitative and operator-dependent  
65 method, MMT is poorly responsive ([Bohannon, 2005](#)). MMT may be used for rough detection  
66 of muscle weakness but not to finely quantify its severity and its evolution over time.

67 Quantitative measurement of muscle strength allows precise temporal monitoring of muscle  
68 strength and enables the use of Z-scores or percentage of predicted values computed from  
69 datasets and predictive equations ([Hogrel et al., 2007](#); [Harbo et al., 2012](#); [Seymour et al.,  
70 2010](#); [McKay et al., 2016](#)). Portable dynamometers have been demonstrated to be particularly  
71 relevant for quantifying muscle strength at low-cost and ease of use within daily clinical  
72 practice and multicenter research trials. Good agreement has been reported between isometric  
73 strength measurement using hand-held dynamometry (HHD) and the “gold standard”  
74 isokinetic dynamometer ([Stark et al., 2011](#)). However, evaluator strength limits the magnitude  
75 of isometric force that can be measured using HHD ([Deones et al., 1994](#)). For powerful  
76 muscle groups such as the quadriceps, belt-stabilization may be used to improve the reliability  
77 and the range of measurable muscle strength using HHD ([Bohannon et al., 2011](#); [Bohannon et  
78 al., 2012](#); [Bachasson et al., 2014](#)). However stabilized HHD is mostly achieved using home-  
79 made methods that may be imperfectly adapted, may lead to discomfort and are unlikely to be  
80 standardized for repeated testing ([Hansen et al., 2015](#)). Some approaches may also fail to

1  
2  
3 81 provide accurate assessment of muscle strength in the weakest patients, partly due to design  
4  
5 82 flaws and metrological limitations inherent in the hardware used, as typically observed in  
6  
7  
8 83 patients with muscle dystrophy for instance (Servais et al., 2013).

9  
10 84 The current manuscript introduces a novel portable device prototype (namely, the MyoQuad)  
11  
12 85 for the assessment and monitoring of isometric knee extension strength that may be used in  
13  
14 86 most clinical setups. This article is organized as follows: description of the device, evaluation  
15  
16  
17 87 of the device in patients including cross-validation with the gold standard, between-day  
18  
19 88 reproducibility of measurements and ability to monitor changes in muscle strength over time  
20  
21 89 with the gold standard method as a reference.  
22  
23  
24 90

## 26 91 **Methods**

### 29 92 **Participants**

31 93 The device was tested in patients with inclusion body myositis enrolled in a natural history  
32  
33 94 study (NCT00898989) and in a pharmacological trial (NCT02481453). The patients were  
34  
35 95 included according to the criteria defined by Benveniste and Hilton-Jones (2010). These  
36  
37  
38 96 studies conformed to the Declaration of Helsinki and were approved by the local ethics  
39  
40 97 committee (CPP-Ile de France VI). All participants gave written informed consent. All tests  
41  
42  
43 98 were performed between April 2013 and April 2017.

### 45 99 **Description of the device for the assessment of isometric knee extension strength**

47 100 The device used in the present study was a first-generation prototype. The MyoQuad was  
48  
49 101 specifically designed for the assessment of maximal isometric strength, even in very weak  
50  
51 102 individuals. It embeds a high precision load cell (Interface SML-300, Scottsdale, Arizona,  
52  
53 103 USA) and electronic board dedicated to signal acquisition and processing, wireless signal  
54  
55  
56 104 transmission (Bluetooth), and operating-energy controls. The current prototype has a  
57  
58  
59 105 measurement range from 0 to 136 kg with 10 g resolution and 50 g accuracy over the whole  
60

1  
2  
3 106 nominal range. The load cell and the board are included in a 3D-printed case, which can be  
4  
5 107 firmly and securely attached to the structure of any examination bed/table using a clamp (see  
6  
7 108 Figure 1A). A dedicated software was developed allowing the visualization and analysis of  
8  
9 109 the acquired strength signal. The software can be run from a phone/tablet or laptop. One  
10  
11 110 extremity of the load cell is equipped with a hook on which a strap can be attached (see  
12  
13 111 Figure 1B). Other interfaces may also be screwed directly onto the load cell for other  
14  
15 112 applications in traction and compression. The MyoQuad device was checked for calibration  
16  
17 113 using strict standardized operating procedures. A set of M3 class masses from 0.2 to 50 kg  
18  
19 114 was used for calibration. The calibration was checked every week, then every month after 6  
20  
21 115 months, then every 2 months after 12 months. The metrological properties of the device were  
22  
23 116 always within the requirements (50-g accuracy over the whole range of measurement). A  
24  
25 117 typical calibration curve is presented in Figure 2.

### 30 118 **Measurement protocol**

31  
32  
33 119 Subjects were seated on a standard examination table with the hip and knee flexed to 90°. A  
34  
35 120 small dense foam pillow was placed below the tested thigh (see Figure 1.A. and Figure 1.B.),  
36  
37 121 so that the leg was vertical in order to avoid any effects of gravity effect, which can be  
38  
39 122 detrimental for the assessment of very weak patients. The desired strap location (lower part of  
40  
41 123 the strap above the medial malleolus) and the medial tibiofemoral joint space were marked on  
42  
43 124 the skin. The distance between the two marks i.e. the lever arm, was carefully measured to the  
44  
45 125 nearest half-centimeter using a measuring tape (Figure 2) to compute the torque as force  $\times$   
46  
47 126 lever arm, allowing direct comparison between methods (MyoQuad vs. isokinetic  
48  
49 127 dynamometer). The ankle strap was then fixed and attached to the dynamometer. The height  
50  
51 128 of the table was adjusted to ensure the strap was horizontal. Participants were asked to keep  
52  
53 129 their hands on their thighs. The evaluator secured the patient at the thigh and shoulder levels  
54  
55 130 on the tested side in order to limit compensatory movements.  
56  
57  
58  
59  
60

### 131 **Isokinetic dynamometer**

132 Participants sat (85° hip flexion) on an ergometer (Biodex System 3 Pro, Biodex Medical,  
133 Shirley, NY, USA). The upper body was stabilized with straps across the thorax and the  
134 abdomen. Knee joint axis of rotation was aligned with the measurement axis of the system.  
135 The thigh was strapped around the mid-thigh of the leg to be tested. The knee angle was  
136 placed at 90° to cancel the effect of gravity. All measurements were performed in an isometric  
137 mode.

### 138 **Assessment of maximal voluntary isometric knee extension voluntary torque (MVIT)**

139 Patients were instructed to perform maximal effort during a static knee extension and to limit  
140 countermovement. Three maximal voluntary contractions were recorded for each  
141 dynamometer. A fourth and possibly fifth trial were performed if the value reached during the  
142 last trial was higher than the preceding ones, or if the difference between trials was greater  
143 than 10%. Strong verbal encouragements were provided to the subjects. For MyoQuad  
144 measurements, the patient was stabilized using one hand on the thigh and the other on the  
145 shoulder on the measured side. Measurements were performed on both sides. The maximal  
146 value from all trials was used for analyses.

### 147 **Data analysis**

148 Torque were expressed as absolute values and as percentage of predictive values using  
149 previous published equations ([Hogrel et al., 2007](#)).

### 150 **Statistics**

151 Data within text and tables are shown as mean  $\pm$  standard deviation (SD) or mean [lower 95%  
152 confidence interval, upper 95% confidence interval]. The assumptions of normality and  
153 sphericity were confirmed using the D'Agostino K-squared and Mauchly tests, respectively.  
154 For cross-validation and between-day reproducibility, change in mean (CIM) and paired t-  
155 tests were used for detection of systematic bias. Standard error of measurement (SEM) was



1  
2  
3 156 used to study absolute reliability. Relative reliability was assessed using intra-class correlation  
4  
5 157 coefficients (ICC<sub>2,1</sub>). Regression analysis and Bland–Altman plots were also performed.  
6  
7 158 Individual coefficients of correlation were computed for between-day measurements and a  
8  
9  
10 159 paired sample t-test was used to compare individual coefficients of correlation between  
11  
12 160 methods. The same approach was used to compare change between methods at follow-up. In  
13  
14 161 addition, a two-way ANOVA (timepoint × method) was used to compare methods. Tukey’s  
15  
16 162 honest significant difference post-hoc tests were conducted when a significant main and/or  
17  
18 163 interaction effect was found. Least significant difference was defined as SEM × 2 and  
19  
20 164 outcome at follow-up was defined as impaired, unchanged, and improved. A Fisher exact  
21  
22 165 probability test was used to compare contingency tables of outcomes at follow-up. All  
23  
24 166 analyses were performed in the computing environment R Version 3.2.3. Statistical  
25  
26 167 significance was set at  $p < 0.05$  for all tests.  
27  
28  
29  
30  
31 168

## 32 33 169 **Results**

34  
35  
36 170 A total of 56 patients (age =  $67 \pm 9$  years) with inclusion body myositis were included. Thirty-  
37  
38 171 three patients were assessed for between-day reproducibility. Thirty-two of which were  
39  
40 172 reassessed after 6 and 12 months. Amongst them, 29 were tested using both methods. The  
41  
42 173 reason for the smaller number of patients at follow-up was time constraints or unavailability  
43  
44 174 of the MyoQuad. Ultimately, a total of 287 observations using both methods were gathered.  
45  
46 175 Agreement of methods are summarized in Table 1 and Figure 3. The MVIT measured using  
47  
48 176 the MyoQuad was significantly lower than the MVIT measured using the Biodex. Between-  
49  
50 177 day reproducibility results for both methods are displayed in Table 2 and Figure 4. No  
51  
52 178 systematic bias was detected and least significant difference was 4.9 and 5.3 Nm for the  
53  
54 179 MyoQuad and the Biodex, respectively. Individual coefficients of variation for between-day  
55  
56 180 measurements were  $5.4 \pm 7.4$  % and  $6.7 \pm 6.6$  % using MyoQuad and the Biodex with no  
57  
58  
59  
60

1  
2  
3 181 significant difference between methods (mean of the differences = -1.4 Nm; 95% CI: [-3.7,  
4  
5 182 0.9] Nm;  $p = 0.26$ ).  
6  
7  
8 183 Change in MVIT at 6 and 12 months using both methods is shown in Figure 5. When  
9  
10 184 performed using absolute values (at baseline, 6, and 12 months), ANOVA showed significant  
11  
12 185 main effects of method and time (both  $p < 0.01$ ) and no significant timepoint  $\times$  method  
13  
14 186 interaction ( $p = 0.19$ ) (Figure 5.A). When performed using absolute changes at 6 and 12  
15  
16 187 months, ANOVA showed significant main effects of method and time (both  $p < 0.05$ ) and no  
17  
18 188 significant timepoint  $\times$  method interaction ( $p = 0.46$ ) (Figure 5.B). Variability in changes  
19  
20 189 between methods at follow-up is displayed in Table 3. A contingency table of outcomes at  
21  
22 190 follow-up is shown in Table 4.  
23  
24  
25  
26 191

## 27 28 29 192 **Discussion**

30  
31 193 The aim of this study was to introduce a novel device for the assessment of isometric strength  
32  
33 194 of knee extensors, for use in most clinical environments. Agreement with the gold standard,  
34  
35 195 between-day reliability, and the ability of the device to monitor changes in muscle strength  
36  
37 196 over time compared to the gold standard method as a reference were investigated. Main  
38  
39 197 results are as follows: i) the device demonstrates excellent metrological accuracy, ii)  
40  
41 198 measurements obtained using the device exhibit excellent agreement with the gold standard,  
42  
43 199 iii) reliability of measurements obtained using the device was excellent and comparable to  
44  
45 200 results obtained using the gold standard, iii) change in strength over time was similar using  
46  
47 201 the device and the gold standard.  
48  
49  
50

51  
52 202 The MyoQuad device was developed in order to conveniently assess quadriceps strength  
53  
54 203 within routine clinical practice, including in very weak patients. This may be commonly  
55  
56 204 performed using HHD, which, however, presents several limitations. In very strong patients,  
57  
58 205 the evaluator may have difficulties in maintaining the dynamometer in a steady hold, whereas  
59  
60

1  
2  
3 206 the influence of the evaluator may be too important in the weakest patients leading to possible  
4  
5 207 large relative errors. Fixed dynamometers are attractive to tackle these limitations (Mentiplay  
6  
7 208 et al., 2015). However, muscle strength may be improperly or even impossible to assess if the  
8  
9 209 device is improperly designed. For instance, within a recent therapeutic trial in IBM, the  
10  
11 210 system was designed in a way that patients had to carry the weight of the strain gauge before  
12  
13 211 strength produced could be actually measured. As a result, knee extensor strength could not  
14  
15 212 be measured in 3 out of 12 (25%) patients and the consistency of the measurements in other  
16  
17 213 patients was largely flawed (unpublished results). The design of the proposed device tackles  
18  
19 214 these issues as the MyoQuad is directly secured on a fixed frame. HHD have been repeatedly  
20  
21 215 observed to underestimate knee extension strength compared to isometric measurements using  
22  
23 216 an isokinetic dynamometer (Stark et al., 2011; Martin et al., 2006). This is particularly true in  
24  
25 217 stronger individuals where the evaluator may have difficulties stabilizing the measurement  
26  
27 218 chain (Martin et al., 2006; Bohannon et al., 2012). The high agreement between  
28  
29 219 measurements performed using the MyoQuad and the Biodex support that fixed dynamometry  
30  
31 220 improves the robustness of assessments through improved comfort and stability. These data  
32  
33 221 are in line with previous work reporting higher consistency of measurements using a modified  
34  
35 222 procedure of stabilized HHD as compared to standard HHD (Kim et al., 2014; Hansen et al.,  
36  
37 223 2015).  
38  
39 224 Our data shows a low SEM < 8.5 % Nm and high ICC > 0.98 for between-day reproducibility  
40  
41 225 when using the MyoQuad. This was similar to that observed using the Biodex (SEM was <  
42  
43 226 10.0% and ICC was > 0.98). We also reported similar individual coefficients of variation for  
44  
45 227 between-day measurement using the MyoQuad and the Biodex. This high reproducibility  
46  
47 228 yielded similar least significant change using both methods. These data are in line with  
48  
49 229 previous reports that have investigated between-day reliability using gold standard methods  
50  
51 230 (Ruschel et al., 2015; Kean et al., 2010). Importantly, our data showed no significant  
52  
53  
54  
55  
56  
57  
58  
59  
60

1  
2  
3 231 difference between methods for monitoring change in MVIT over time (Figure 5) and good  
4  
5 232 agreement when comparing changes at follow-up (Table 3). This was confirmed by consistent  
6  
7 233 classification of strength changes using both methods at follow-up (Table 4). To the best of  
8  
9  
10 234 our knowledge, this is the first report that compares temporal changes in knee extensors using  
11  
12 235 fixed dynamometry and standard isokinetic dynamometry.  
13  
14 236 As this study was only performed in patients with inclusion body myositis, generalizability of  
15  
16 237 findings to other disorders remains to be demonstrated. However, similar findings regarding  
17  
18 238 the reliability of MVIT have been previously reported in various clinical fields (Nuzzo et al.,  
19  
20 239 2019). Volitional maneuvers such as maximal voluntary contraction embraces both peripheral  
21  
22  
23 240 and central factors, which render its estimation variable (Millet et al., 2012). Therefore,  
24  
25 241 observed differences between Biodex and MyoQuad also reflect this variability. Another  
26  
27 242 potential source of error using the MyoQuad is the measurement of the lever arm to compute  
28  
29 243 torque that is circumvented when using torque meter as in standard isokinetic dynamometers  
30  
31 244 like the Biodex (Ruschel et al., 2015).  
32  
33  
34  
35  
36  
37

245

## 246 **Conclusions**

247 Measurement of maximal voluntary isometric knee extension torque using the MyoQuad  
248 offers a cost-effective, portable and immediate alternative for the routine measurement of  
249 maximal voluntary isometric contraction of the quadriceps by offering comfort and stability  
250 that cannot be provided using hand-held dynamometry. It may be used for both baseline and  
251 follow-up assessments of muscle strength and may also be used to assess other muscle groups  
252 (e.g. knee flexion, shoulder abduction) using proper patient positioning and adapted  
253 interfaces. Altogether, our results support the adoption of quantitative muscle strength  
254 assessment using fixed yet flexible dynamometry within routine clinical practice and  
255 multicenter trials.

1  
2  
3 256  
45  
6 257 **Acknowledgments**  
78 258 We gratefully thank all the patients who participated in this study. This study was supported by  
9  
10 259 the *Association Française contre les Myopathies* (AFM). The authors are grateful to Simone  
11  
12  
13 260 Birnbaum for English editing.  
14

15 261

16  
17  
18 262 **ORCID iDs**  
1920 263 Jean-Yves Hogrel: <https://orcid.org/0000-0003-0045-7505>  
2122 264 Olivier Benveniste: <https://orcid.org/0000-0002-1167-5797>  
2324 265 Damien Bachasson: <https://orcid.org/0000-0001-6335-9916>  
25  
2627 266  
28  
2930 267 **References**  
3132  
33 268 Bachasson D, Villiot-Danger E, Verges S, Hayot M, Perez T, Chambellan A and Wuyam B  
34  
35 269 2014 [Maximal isometric voluntary quadriceps strength assessment in COPD] *Revue*  
36  
37  
38 270 *des Maladies Respiratoires* **31** 765-70  
3940 271 Benveniste O and Hilton-Jones D 2010 International Workshop on Inclusion Body Myositis  
41  
42 272 held at the Institute of Myology, Paris, on 29 May 2009 *Neuromuscul Disord* **20** 414-  
43  
44 273 21  
4546  
47 274 Bohannon R W 2005 Manual muscle testing: does it meet the standards of an adequate  
48  
49 275 screening test? *Clinical Rehabilitation* **19** 662-7  
5051 276 Bohannon R W, Bubela D J, Wang Y C, Magasi S R and Gershon R C 2011 Adequacy of belt-  
52  
53 277 stabilized testing of knee extension strength *Journal of Strength and Conditioning*  
54  
55 278 *Research* **25** 1963-7  
56  
57  
58  
59  
60

- 1  
2  
3 279 Bohannon R W, Kindig J, Sabo G, Duni A E and Cram P 2012 Isometric knee extension force  
4  
5 280 measured using a handheld dynamometer with and without belt-stabilization *Physiother*  
6  
7 281 *Theory Pract* **28** 562-8
- 8  
9  
10 282 Deones V L, Wiley S C and Worrell T 1994 Assessment of quadriceps muscle performance by  
11  
12 283 a hand-held dynamometer and an isokinetic dynamometer *Journal of Orthopaedic &*  
13  
14 284 *Sports Physical Therapy* **20** 296-301
- 15  
16  
17 285 Garcia-Hermoso A, Cavero-Redondo I, Ramirez-Velez R, Ruiz J R, Ortega F B, Lee D-C and  
18  
19 286 Martinez-Vizcaino V 2018 Muscular Strength as a Predictor of All-Cause Mortality in  
20  
21 287 an Apparently Healthy Population: A Systematic Review and Meta-Analysis of Data  
22  
23 288 From Approximately 2 Million Men and Women *Arch Phys Med Rehabil* **99** 2100-13.e5
- 24  
25  
26 289 Hansen E M, McCartney C N, Sweeney R S, Palimenio M R and Grindstaff T L 2015 Hand-  
27  
28 290 held Dynamometer Positioning Impacts Discomfort During Quadriceps Strength  
29  
30 291 Testing: A Validity and Reliability Study *Int J Sports Phys Ther* **10** 62-8
- 31  
32  
33 292 Harbo T, Brincks J and Andersen H 2012 Maximal isokinetic and isometric muscle strength of  
34  
35 293 major muscle groups related to age, body mass, height, and sex in 178 healthy subjects  
36  
37 294 *European Journal of Applied Physiology* **112** 267-75
- 38  
39  
40 295 Hogrel J Y, Ollivier G and Desnuelle C 2006 [Manual and quantitative muscle testing in  
41  
42 296 neuromuscular disorders. How to assess the consistency of strength measurements in  
43  
44 297 clinical trials?] *Rev Neurol (Paris)* **162** 427-36
- 45  
46  
47 298 Hogrel J Y, Payan C A, Ollivier G, Tanant V, Attarian S, Couillandre A, Dupeyron A,  
48  
49 299 Lacomblez L, Doppler V, Meininger V, Tranchant C, Pouget J and Desnuelle C 2007  
50  
51 300 Development of a French isometric strength normative database for adults using  
52  
53 301 quantitative muscle testing *Archives of Physical Medicine and Rehabilitation* **88** 1289-  
54  
55 302 97  
56  
57  
58  
59  
60

- 1  
2  
3 303 Kean C O, Birmingham T B, Garland S J, Bryant D M and Giffin J R 2010 Minimal detectable  
4  
5 304 change in quadriceps strength and voluntary muscle activation in patients with knee  
6  
7 305 osteoarthritis *Archives of Physical Medicine and Rehabilitation* **91** 1447-51  
8  
9  
10 306 Kim W K, Kim D K, Seo K M and Kang S H 2014 Reliability and validity of isometric knee  
11  
12 307 extensor strength test with hand-held dynamometer depending on its fixation: a pilot  
13  
14 308 study *Ann Rehabil Med* **38** 84-93  
15  
16  
17 309 Martin H J, Yule V, Syddall H E, Dennison E M, Cooper C and Aihie Sayer A 2006 Is hand-  
18  
19 310 held dynamometry useful for the measurement of quadriceps strength in older people?  
20  
21 311 A comparison with the gold standard Bodex dynamometry *Gerontology* **52** 154-9  
22  
23  
24 312 McKay M J, Baldwin J N, Ferreira P, Simic M, Vanicek N, Hiller C E, Nightingale E J,  
25  
26 313 Moloney N A, Quinlan K G, Pourkazemi F, Sman A D, Nicholson L L, Mousavi S J,  
27  
28 314 Rose K, Raymond J, Mackey M G, Chard A, Hubscher M, Wegener C, Fong Yan A,  
29  
30 315 Refshauge K M, Burns J and Norms Project C 2016 1000 Norms Project: protocol of a  
31  
32 316 cross-sectional study cataloging human variation *Physiotherapy* **102** 50-6  
33  
34  
35 317 Mentiplay B F, Perraton L G, Bower K J, Adair B, Pua Y H, Williams G P, McGaw R and  
36  
37 318 Clark R A 2015 Assessment of Lower Limb Muscle Strength and Power Using Hand-  
38  
39 319 Held and Fixed Dynamometry: A Reliability and Validity Study *PLoS One* **10** e0140822  
40  
41  
42 320 Millet G Y, Bachasson D, Temesi J, Wuyam B, Feasson L, Verges S and Levy P 2012 Potential  
43  
44 321 interests and limits of magnetic and electrical stimulation techniques to assess  
45  
46 322 neuromuscular fatigue *Neuromuscul Disord* **22 Suppl 3** S181-6  
47  
48  
49 323 Nuzzo J L, Taylor J L and Gandevia S C 2019 CORP: Measurement of upper and lower limb  
50  
51 324 muscle strength and voluntary activation *J Appl Physiol (1985)* **126** 513-43  
52  
53  
54 325 Ruschel C, Hauptenthal A, Jacomel G F, Fontana Hde B, Santos D P, Scoz R D and Roesler H  
55  
56 326 2015 Validity and reliability of an instrumented leg-extension machine for measuring  
57  
58 327 isometric muscle strength of the knee extensors *Journal of Sport Rehabilitation* **24**  
59  
60

- 1  
2  
3 328 Servais L, Deconinck N, Moraux A, Benali M, Canal A, Van Parys F, Vereecke W,  
4  
5 329 Wittevrongel S, Mayer M, Desguerre I, Maincent K, Themar-Noel C, Quijano-Roy S,  
6  
7 330 Serari N, Voit T and Hogrel J Y 2013 Innovative methods to assess upper limb strength  
8  
9 and function in non-ambulant Duchenne patients *Neuromuscul Disord* **23** 139-48  
10 331  
11  
12 332 Seymour J M, Spruit M A, Hopkinson N S, Nataneek S A, Man W D, Jackson A, Gosker H R,  
13  
14 333 Schols A M, Moxham J, Polkey M I and Wouters E F 2010 The prevalence of  
15  
16 334 quadriceps weakness in COPD and the relationship with disease severity *Eur Respir J*  
17  
18 **36** 81-8  
19 335  
20  
21 336 Stark T, Walker B, Phillips J K, Fejer R and Beck R 2011 Hand-held dynamometry correlation  
22  
23 with the gold standard isokinetic dynamometry: a systematic review *PM R* **3** 472-9  
24 337  
25  
26 338  
27  
28  
29  
30  
31  
32  
33  
34  
35  
36  
37  
38  
39  
40  
41  
42  
43  
44  
45  
46  
47  
48  
49  
50  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60



339 **Tables**

340 **Table 1. Agreement of measurements obtained using the MyoQuad and the Biodex (n =**  
 341 **52 participants with a total of 283 measurements).**

MyoQuad (Nm)	Biodex (Nm)	CIM (Nm) [95% CI]	P value	ICC [95% CI]	SEM (Nm) [95% CI]
29.46 ± 23.12	31.14 ± 24.68	1.68 [1.06, 2.30]	< 0.001	0.973 [0.966, 0.979]	3.76 [3.47, 4.10]

342 CIM = change in mean; SEM = standard error of measurement; ICC = intra-class correlation  
 343 coefficient.

344

345

346 **Table 2. Test-retest reliability of maximal isometric knee extension voluntary torque using**  
 347 **the MyoQuad and the Biodex (n = 33 participants with a total of 66 measurements).**

Method	Test (Nm)	Retest (Nm)	CIM (Nm) [95% CI]	<i>p</i> value	ICC [95% CI]	SEM (Nm) [95% CI]
MyoQuad	32.20 ± 23.58	31.72 ± 22.78	-0.48 [-1.33, 0.36]	0.258	0.989 [0.982, 0.993]	2.44 [2.08, 2.94]
Biodex	33.36 ± 24.88	32.90 ± 23.98	-0.46 [-1.37, 0.46]	0.323	0.988 [0.981, 0.993]	2.64 [2.25, 3.18]

348 CIM = change in mean; SEM = standard error of measurement; ICC = intra-class correlation  
 349 coefficient.

350

351

1  
2  
3 352 **Table 3. Variability of changes in maximal isometric knee extension voluntary torque at**  
4  
5 353 **follow-up using the MyoQuad and the Biodex (n = 44 participants with a total of 88**  
6  
7 354 **measurements).**  
8  
9

Biodex (Nm)	MyoQuad (Nm)	CIM (Nm) [95% CI]	<i>p</i> value	ICC [95% CI]	SEM (Nm) [95% CI]
-3.15 ± 9.01	-3.17 ± 7.57	-0.02 [-1.29, 1.24]	0.971	0.756 [0.648, 0.836]	4.22 [3.68,4.96]

10  
11  
12  
13  
14  
15  
16 355 CIM = change in mean; ICC = intra-class correlation coefficient; SEM = standard error of  
17  
18 356 measurement.  
19  
20  
21

22 357

23  
24  
25 358

26  
27  
28 359  
29  
30  
31  
32  
33  
34  
35  
36  
37  
38  
39  
40  
41  
42  
43  
44  
45  
46  
47  
48  
49  
50  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60

360 **Table 4. Contingency table illustrating classified changes in strength using the MyoQuad**  
 361 **and the Biodex.**

	<i>6 months</i>			<i>12 months</i>		
<b>Progression</b>	<b>MyoQuad</b>	<b>Biodex</b>	<b>% match</b>	<b>MyoQuad</b>	<b>Biodex</b>	<b>% match</b>
<b>Impaired</b>	13/44	11/44	85%	13/44	15/44	87%
<b>Unchanged</b>	29/44	29/44	100%	29/44	28/44	97%
<b>Improved</b>	2/44	4/44	50%	2/44	1/44	50%

362 Least significant change determined from between-day reliability was used to classify changes  
 363 in strength after 6 and 12 months.

364

365

## 366 **Figure legends**

367 **Figure 1. Patient installation and device.** Close-up view of the device paired with tablet  
368 computer (A); Close-up view of the device attached to table legs with round (B) or  
369 rectangular section (C); Overview of the setup with one participant and stabilization by one  
370 evaluator (D). A small pillow is inserted under the distal part of the thigh to ensure the thigh is  
371 horizontal.

372  
373 **Figure 2. Typical calibration curve.** The dashed line represents the identity line, and the  
374 solid line indicates the linear regression line.

375  
376 **Figure 3. Agreement of measurements obtained using the MyoQuad *versus* the Biodex.**  
377 **Bland–Altman plots (A) and regression analysis (B) of measurements obtained using the**  
378 **MyoQuad and the Biodex.** In A, the solid line indicates the mean difference between the  
379 measurements and dashed lines the limits of agreement. In B, the dashed line represents the  
380 identity line, and the solid line indicates the linear regression line.


381  
382 **Figure 4. Between-day reproducibility of measurements obtained using the MyoQuad**  
383 **and the Biodex. Bland–Altman plots (A, C) and regression analysis (B, D) for between-**  
384 **day reliability of measurements obtained using the MyoQuad and the Biodex,**  
385 **respectively.** In A and C, the solid line indicates the mean difference between the  
386 measurements and the dashed line indicates the limit of agreements. In B and D, the dashed  
387 line represents the identity line, and the solid line indicates the linear regression line.  
388 Logarithmic scales are used for better data visualization.

389

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20  
21  
22  
23  
24  
25  
26  
27  
28  
29  
30  
31  
32  
33  
34  
35  
36  
37  
38  
39  
40  
41  
42  
43  
44  
45  
46  
47  
48  
49  
50  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60


390 **Figure 5. Change in torque over time using the MyoQuad and the Biodex.** Absolute (A)  
391 values and change (B) in knee extensor strength over time.  
392

393 Figure 1

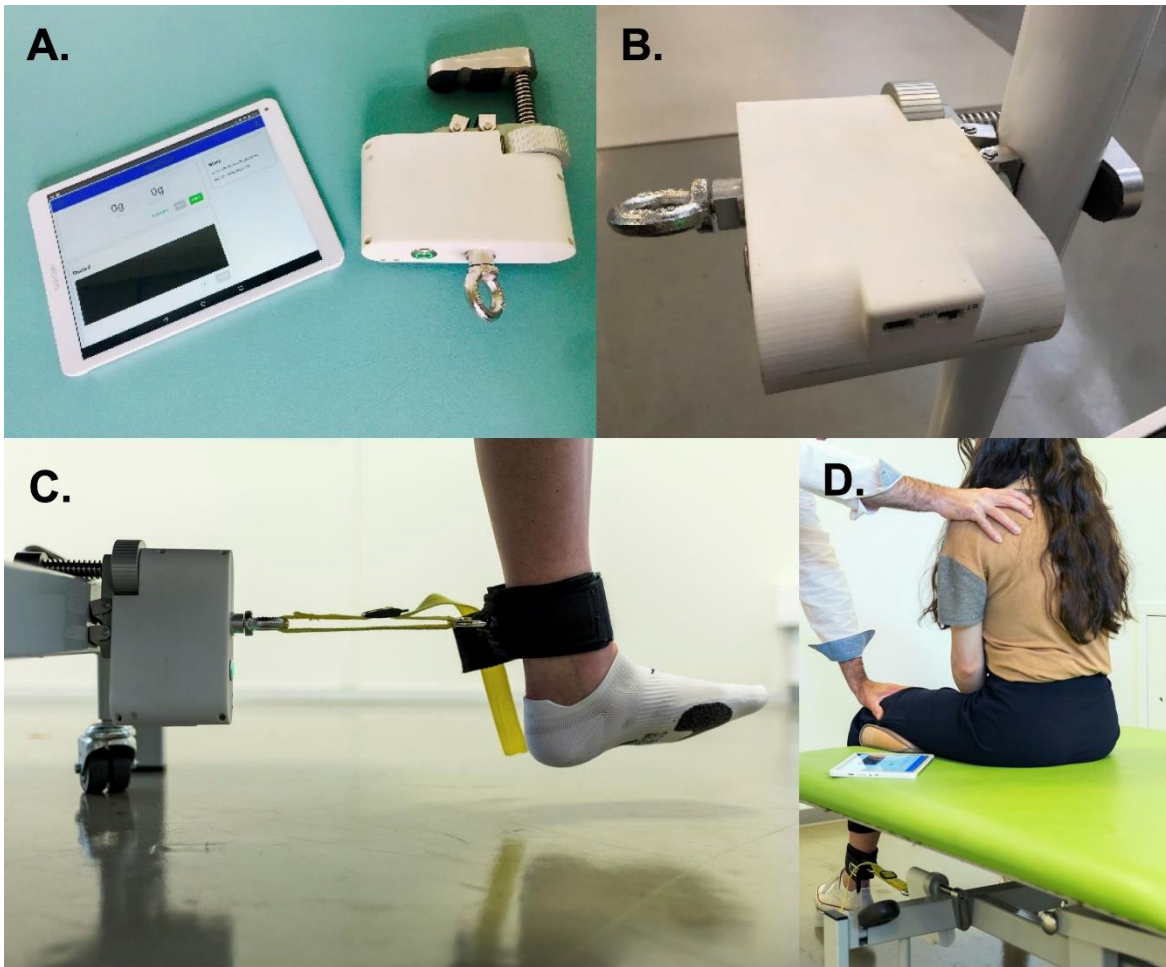

394  
395

396 Figure 2

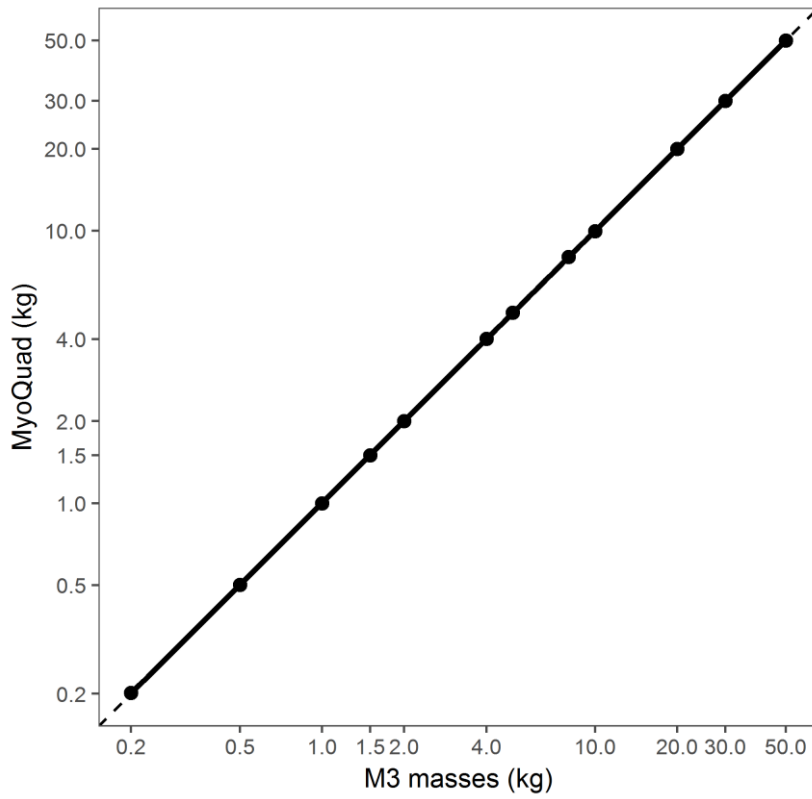


397

398




399 Figure 3

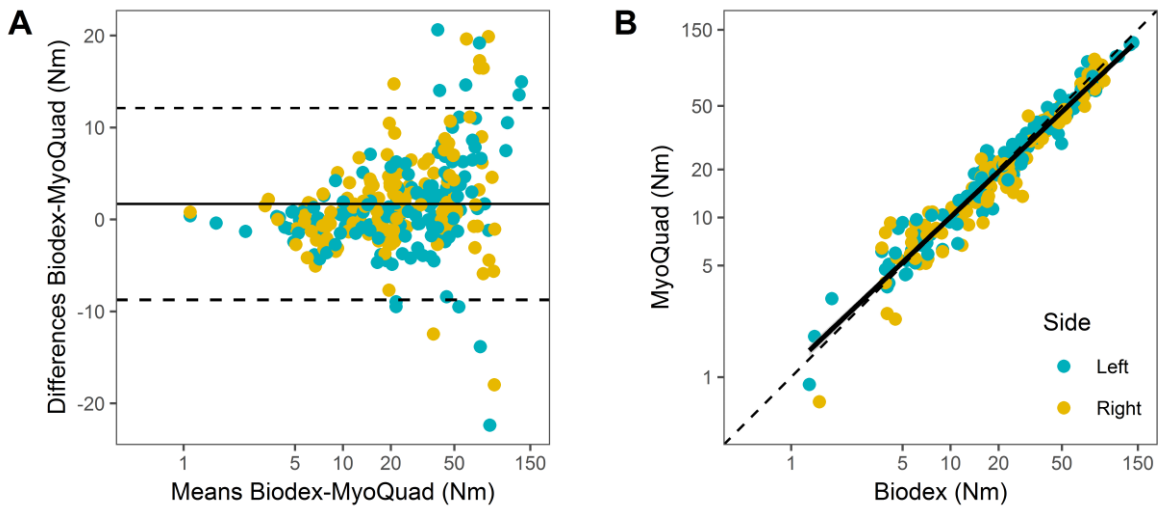

400

401


402 Figure 4

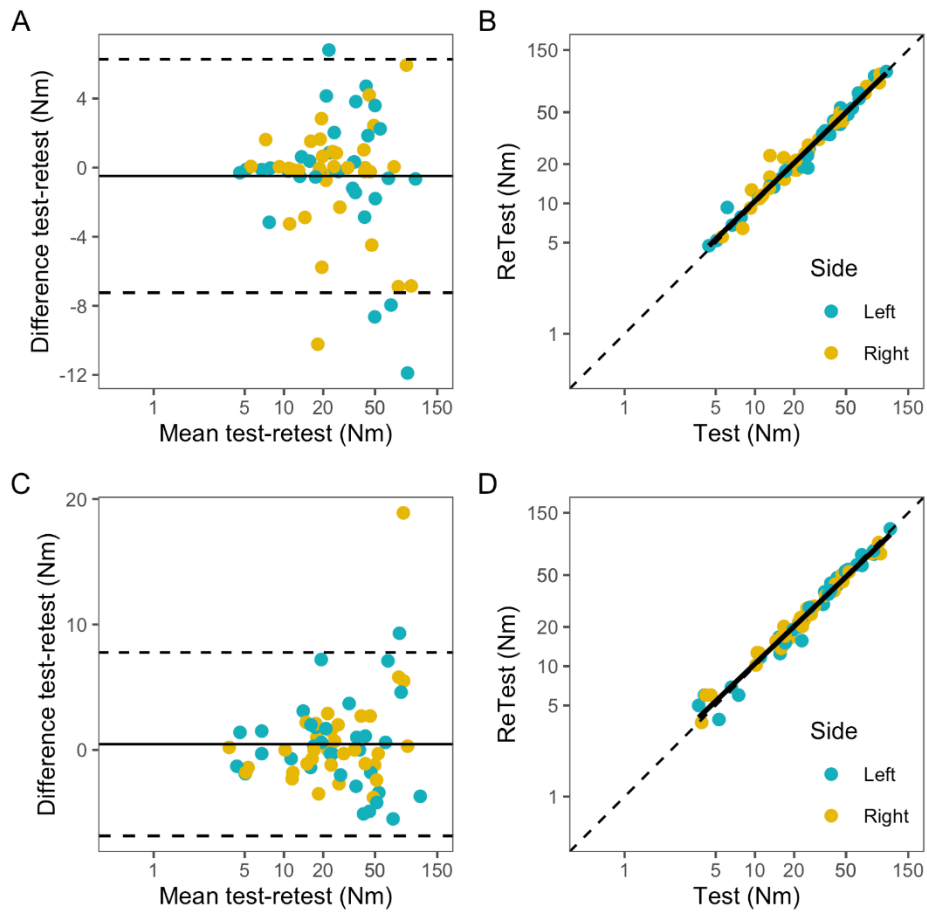

403

404

405 Figure 5

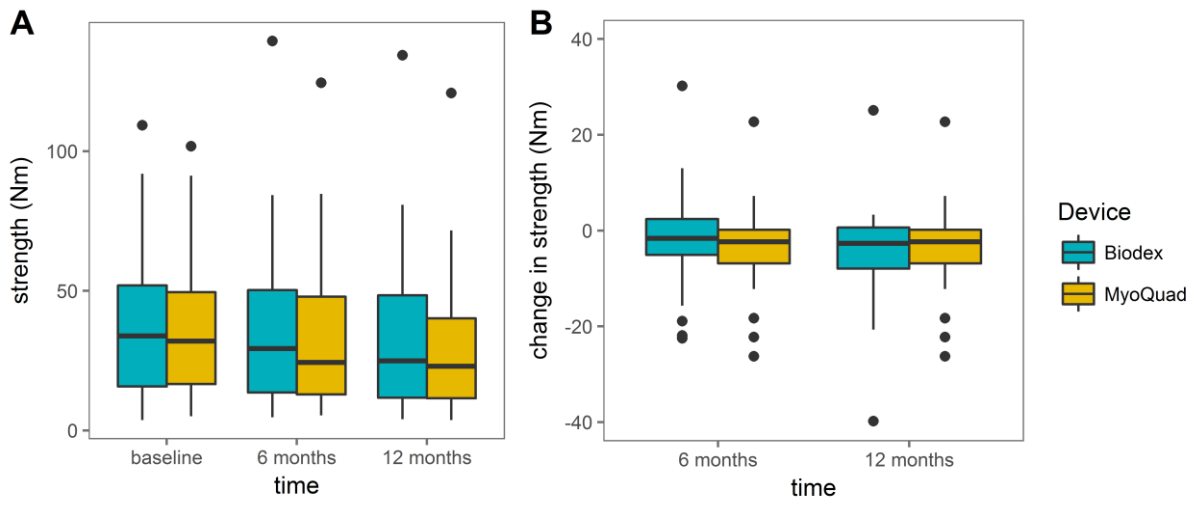

406