



**HAL**  
open science

## Si Traceable High Precision Spectroscopy Of Ozone Using A Quantum Cascade Laser At 9.5 Micrometer

Hadj Elandaloussi, Nicolas Cahuzac, Maxime Leuliet, P. Marie-Jeanne, C. Rouillé, Thomas Zanon-Willette, M. Manceau, O. Lopez, B. Darquié, M. Abgrall, et al.

► **To cite this version:**

Hadj Elandaloussi, Nicolas Cahuzac, Maxime Leuliet, P. Marie-Jeanne, C. Rouillé, et al.. Si Traceable High Precision Spectroscopy Of Ozone Using A Quantum Cascade Laser At 9.5 Micrometer. Congrès des 150 ans de la Société Française de Physique, Jul 2023, Paris, France. hal-04421778

**HAL Id: hal-04421778**

**<https://hal.sorbonne-universite.fr/hal-04421778>**

Submitted on 28 Jan 2024

**HAL** is a multi-disciplinary open access archive for the deposit and dissemination of scientific research documents, whether they are published or not. The documents may come from teaching and research institutions in France or abroad, or from public or private research centers.

L'archive ouverte pluridisciplinaire **HAL**, est destinée au dépôt et à la diffusion de documents scientifiques de niveau recherche, publiés ou non, émanant des établissements d'enseignement et de recherche français ou étrangers, des laboratoires publics ou privés.

# SI TRACEABLE HIGH PRECISION SPECTROSCOPY OF OZONE USING A QUANTUM CASCADE LASER AT 9.5 MICROMETER



LERMA



SYRTE



H. Elandaloussi<sup>1</sup>, N. Cahuzac<sup>1,2</sup>, M. Leuliet<sup>1</sup>, P. Marie-Jeanne<sup>1</sup>, C. Rouillé<sup>1</sup>, T. Zanon-Willette<sup>1</sup>, M. Manceau<sup>2</sup>, O. Lopez<sup>2</sup>, B. Darquié<sup>2</sup>, M. Abgrall<sup>3</sup>, C. Janssen<sup>1</sup>

<sup>1</sup> LERMA, Sorbonne Université, Observatoire de Paris, PSL Université, CNRS


<sup>2</sup> LPL, Université Sorbonne Paris Nord (Univ Paris 13), CNRS

<sup>3</sup> LNE-SYRTE, Sorbonne Université, Observatoire de Paris, PSL Université, CNRS

At Sorbonne-Université, we have developed a SI traceable mid-infrared QCL spectrometer for the investigation of ozone and other molecules of atmospheric and astrophysical interest. Ozone, in particular, has unresolved issues in the mid-IR spectral region at 9.5  $\mu\text{m}$ , where large uncertainties and inconsistencies in ozone broadening [1] and pressure shift [2] parameters exist. There is also the question of appropriately representing molecular line shapes [3]. Following previous work [4, 5], we have implemented a laser stabilisation scheme based on an optical frequency comb (OFC) referenced to the international system of units (SI) via an optical fiber which links to the REFIMEVE network [6]. To compare the QCL at 31 THz to a reference laser frequency comb at 193 THz (SI traceable), a sum frequency generation (SFG) scheme between the QCL and an OFC at 162 THz in an oriented patterned GaAs crystal is implemented.

## Frequency control of the Quantum Cascade Laser


To control the QCL frequency emission around 31 THz, we sum its frequency with an optical-frequency-comb (OFC) at 162 THz to produce an optical frequency comb (OFC) at 194 THz. The sum frequency  $f_{\text{sig}}$  is compared to a SI traceable optical frequency comb at 193 THz, noted  $f_r$ . Frequencies are fixed by the controlled repetition rate frequency  $f_{\text{rep}}$  and the frequency offset  $f_0$ , both SI traceable.

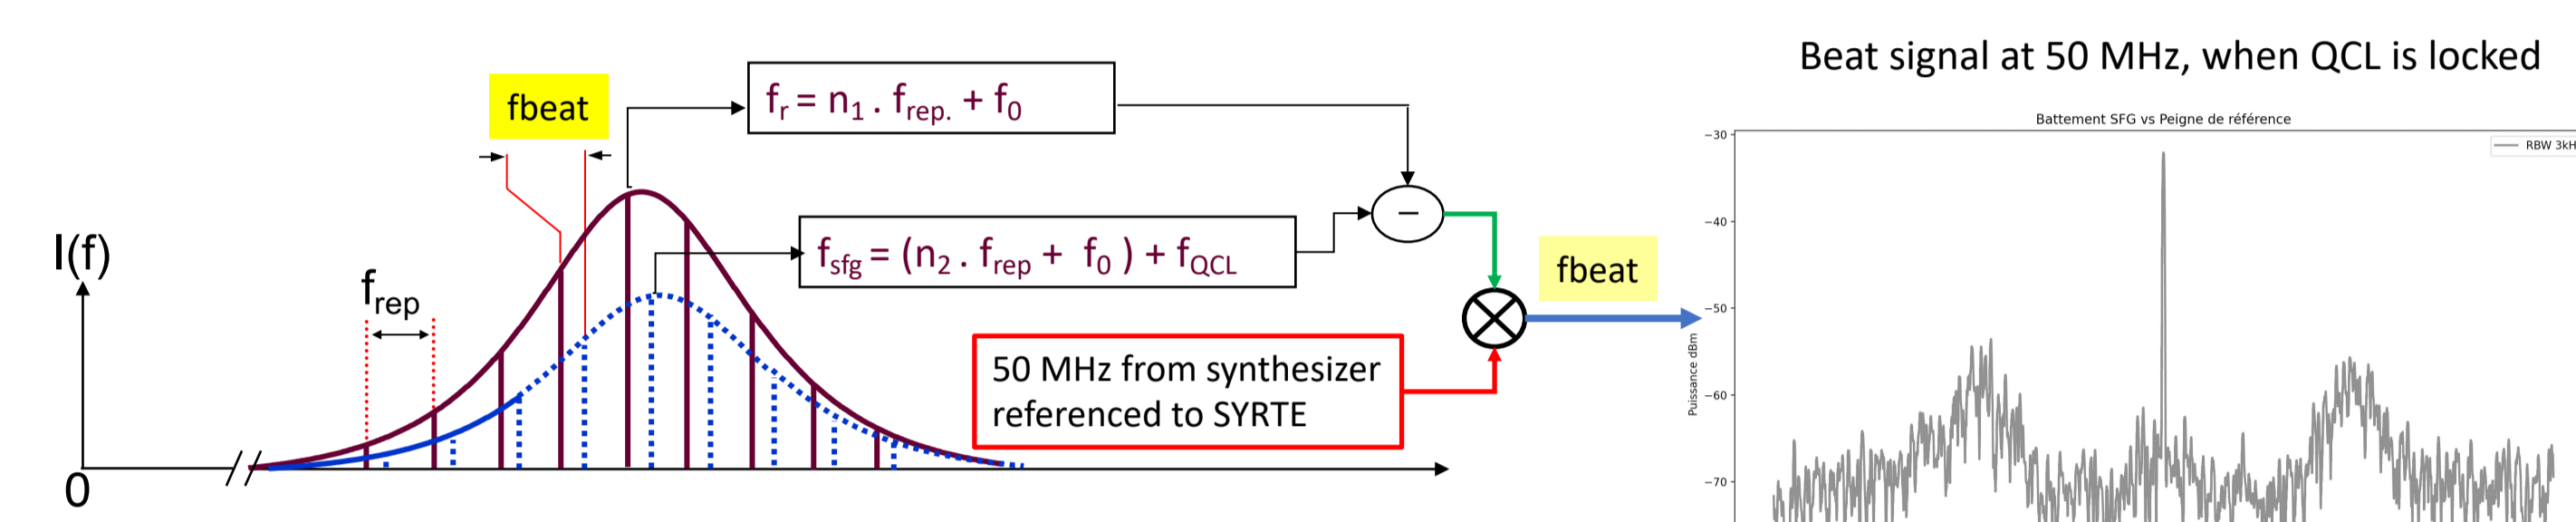


$$f_{\text{sig}} - f_r = f_{\text{beat}} = (n_2 - n_1) f_{\text{rep}} + f_{\text{QCL}}; (n_1 - n_2) \text{ is an integer } \sim 125 \text{ 847.}$$

The  $f_{\text{rep}}$  around 250 MHz is controlled by a  $f_{\text{down}} = 20$  MHz synthesizer as:  $f_{\text{rep}} = 245 \text{ MHz} + \frac{f_{\text{down}}}{4}$



Changing  $f_{\text{down}}$  by 0.1 Hz, alters  $f_{\text{rep}}$  and thus  $f_{\text{QCL}}$  by 3.1 kHz

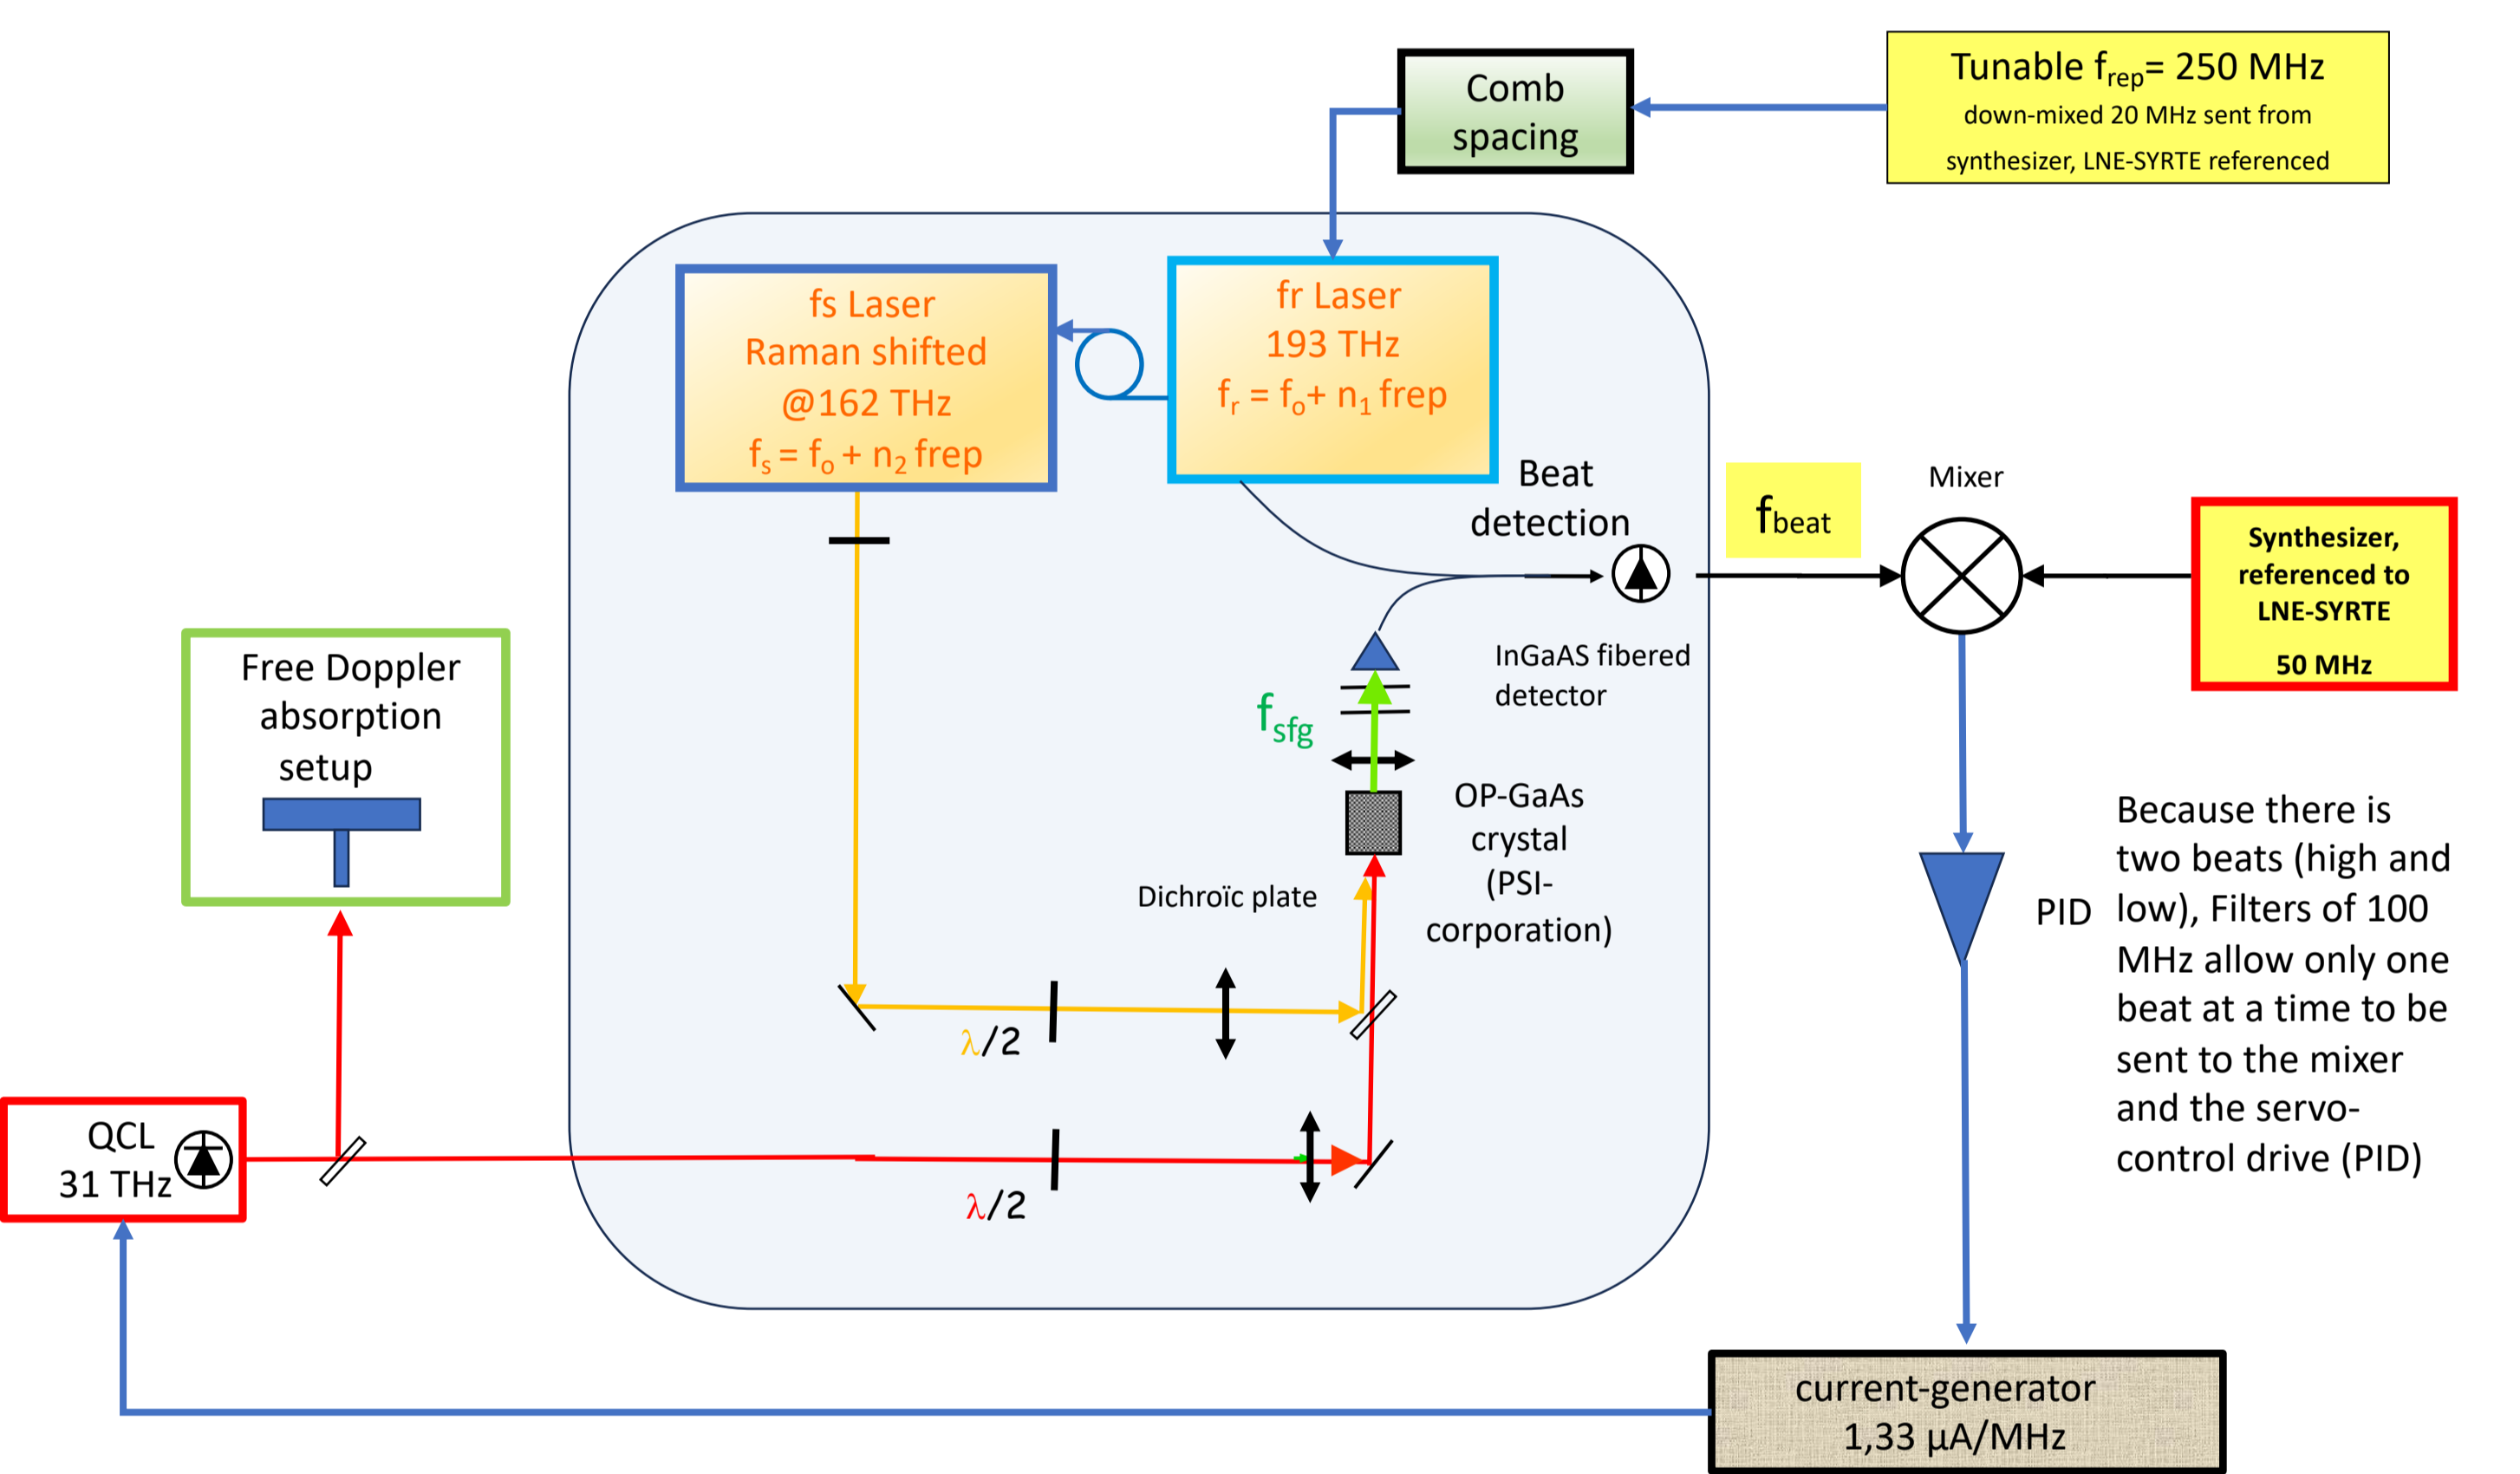


## Ozone, Doppler and Doppler-free spectroscopy setup

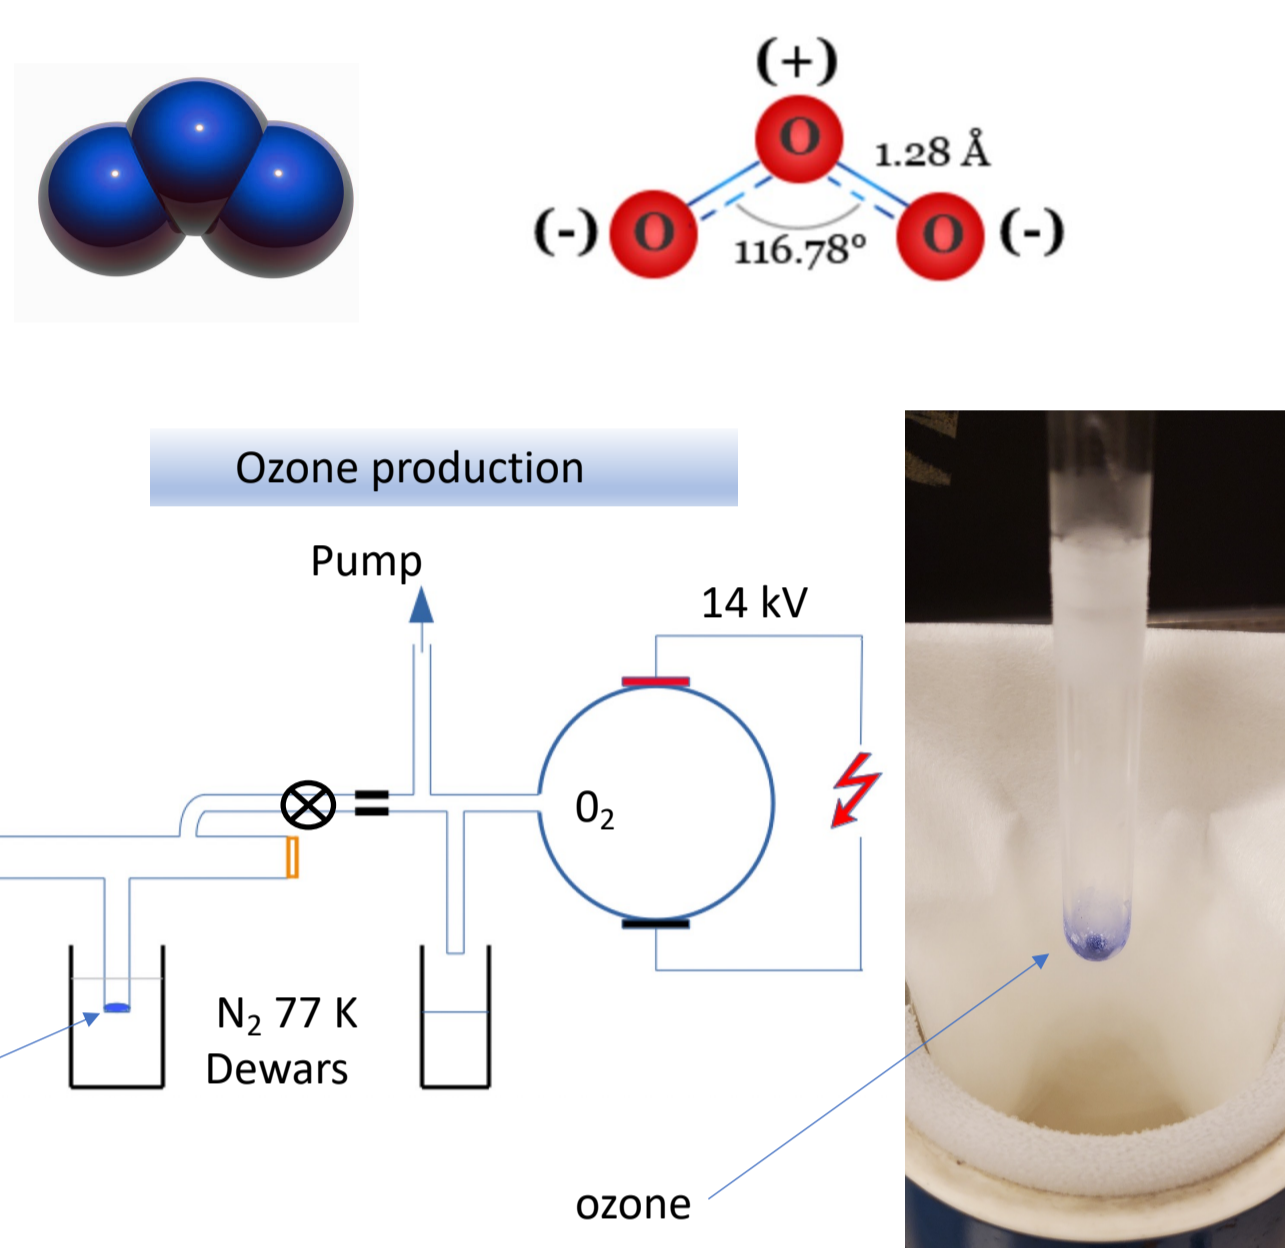


80 cm cell, ozone at 77 K for 2mtorr vapor pressure at 293 K

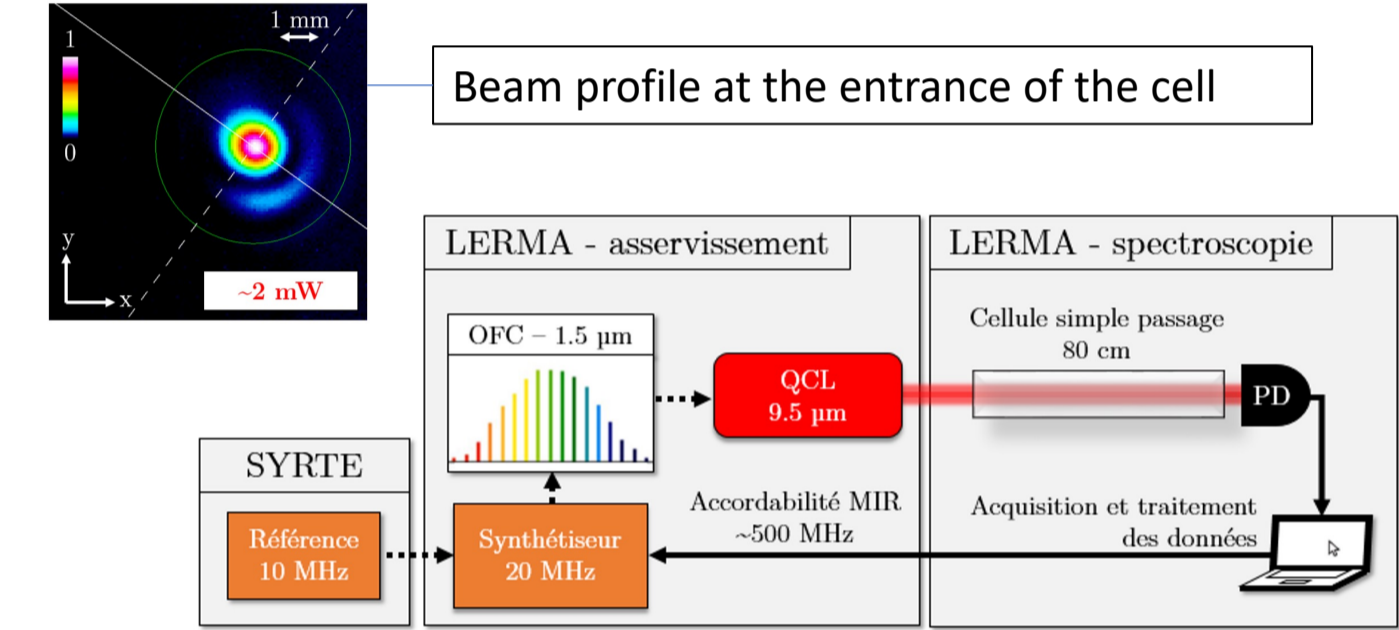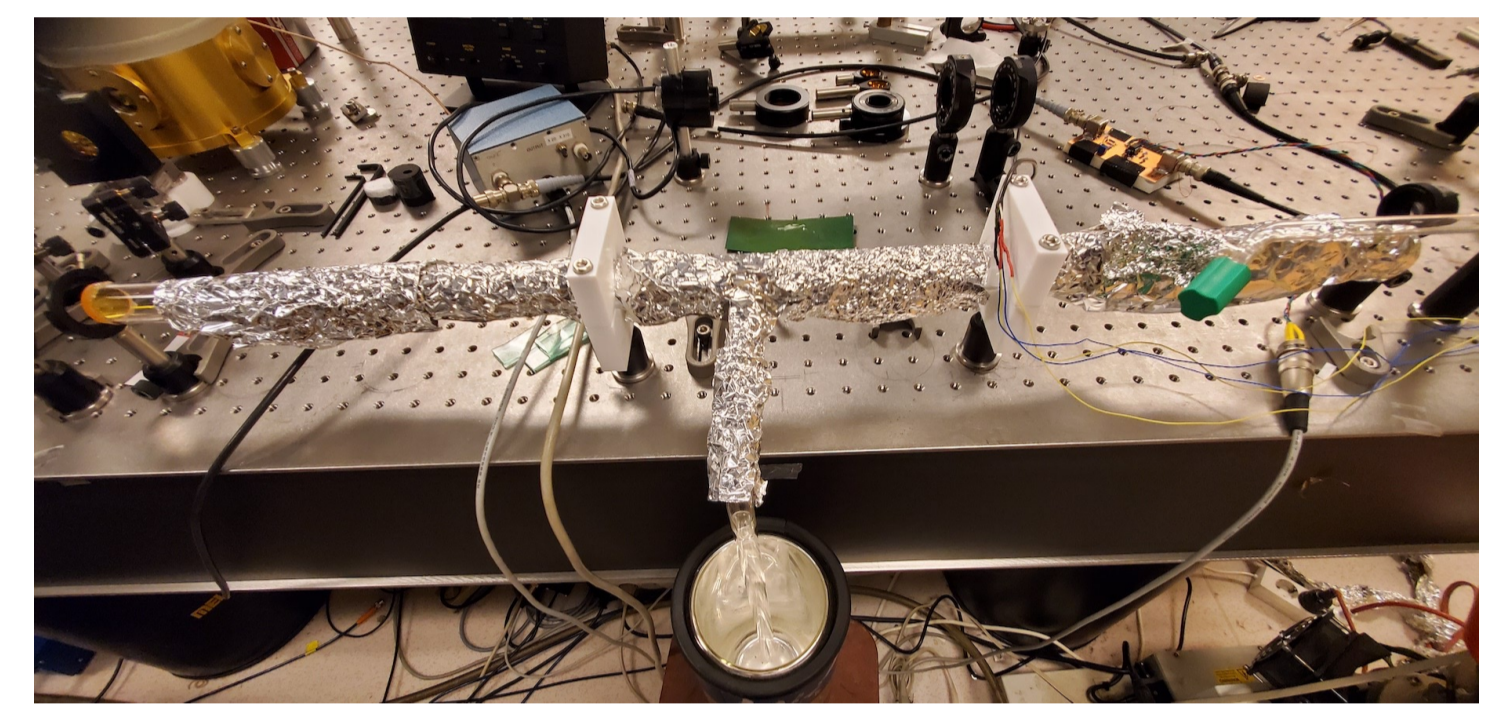


Sum frequency generation laser comb at 1.85  $\mu\text{m}$  + QCL-laser at 9.5  $\mu\text{m}$ . Beat detection using laser comb at 1.55  $\mu\text{m}$

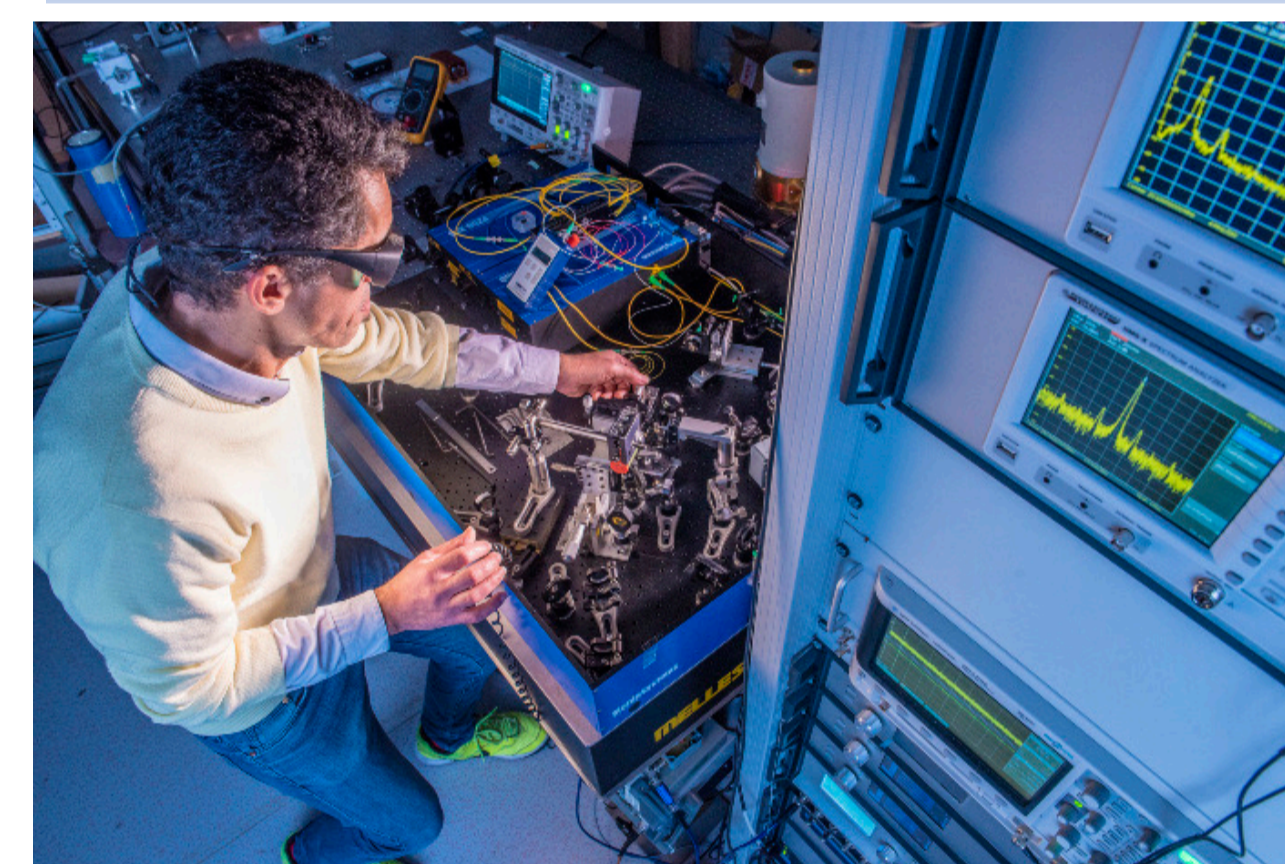

Setup for Doppler free absorption measurements

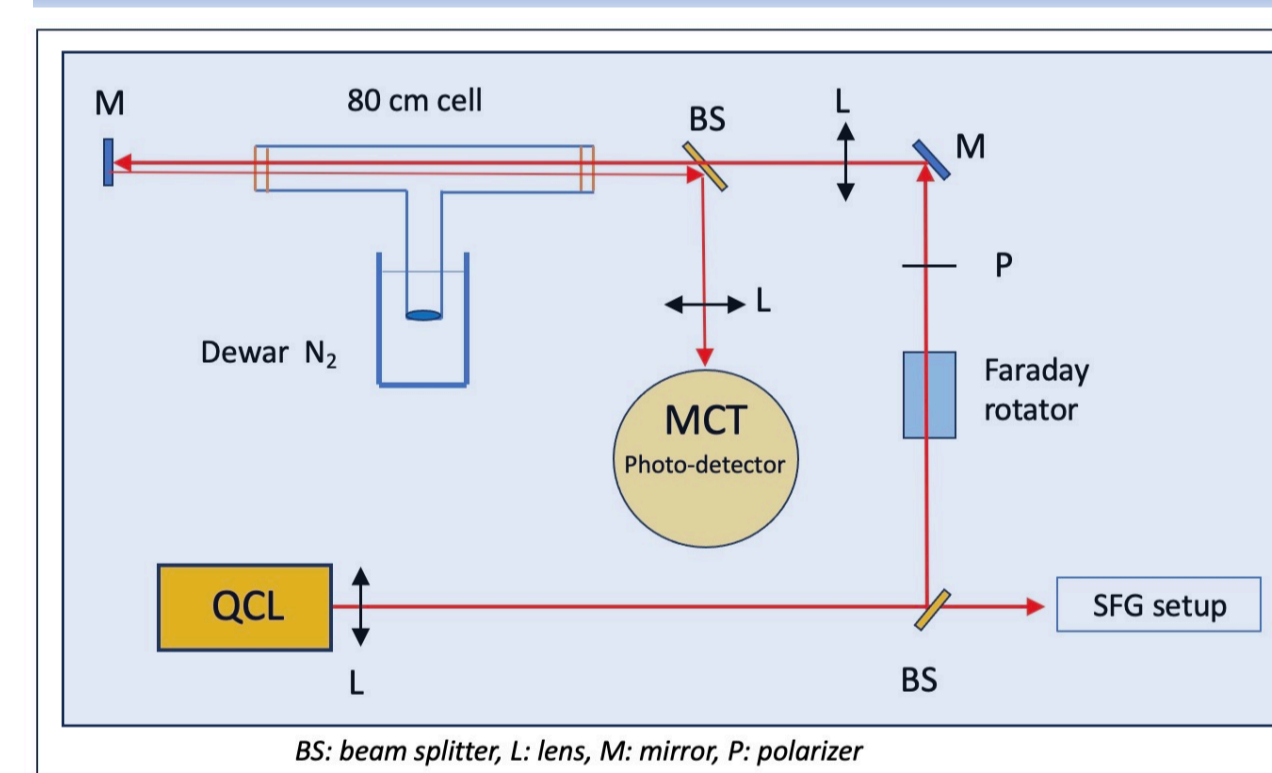


## Spectrometer instrumentation

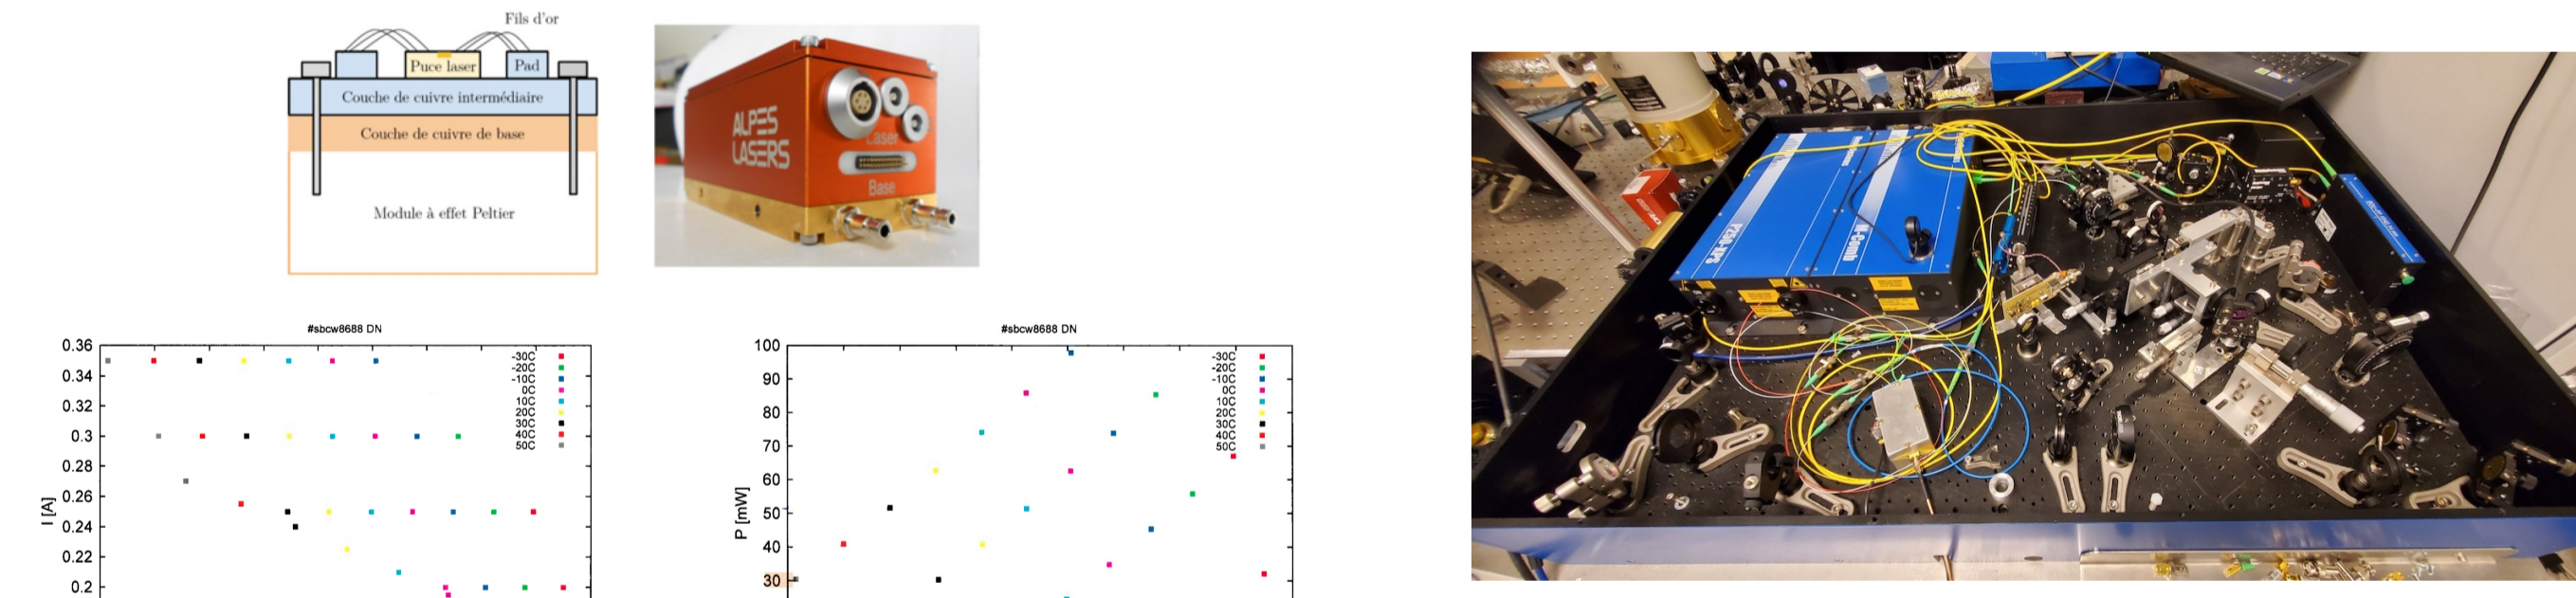

Input current as a function of the single mode emission frequencies and temperature

Output power as a function of the single mode emission frequencies and temperature

Refimeve+ Link from LNE-Syrte-Observatoire de Paris to LERMA-Observatoire de Paris at Sorbonne Université (Jussieu) and other labs

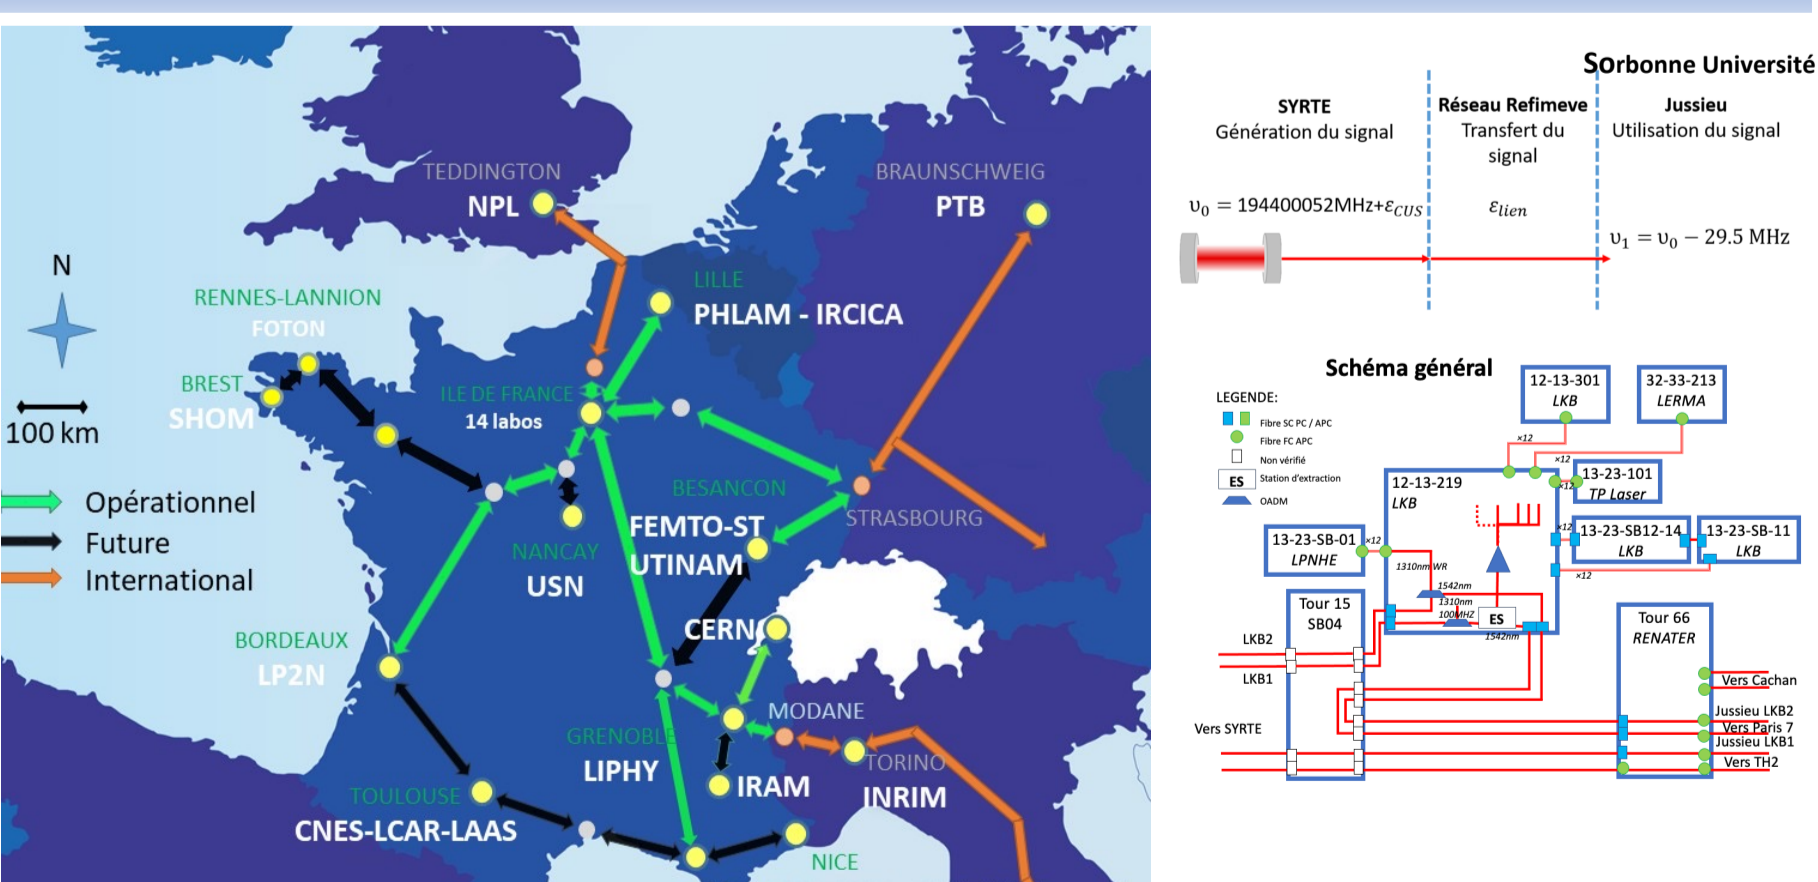

Determination of QCL emission frequency

$$f_{\text{sig}} = n_2 \cdot f_{\text{rep}} + f_0 + f_{\text{QCL}}$$

$$f_r = n_1 \cdot f_{\text{rep}} + f_0$$

$$f_{\text{beat}} = f_{\text{sig}} - f_r$$


The QCL frequency can be written as :

$$f_{\text{QCL}} = (n_1 - n_2) f_{\text{rep}} + f_{\text{beat}}$$


The OFC is controlled by a DDS referenced to the 100 MHz RF (H-maser) signal from LNE-SYRTE, that is distributed via optical fibre to SU-Jussieu for instruments synchronization.

## Ozone spectrum and lines measurement


As a first demonstration of the spectrometer performances, we report on ozone line positions in the  $\nu_3$  R-branch from saturated absorption spectroscopy with line center determinations at the 50 kHz level. This is almost three orders of magnitude more accurate than the current uncertainty index ( $< 10^{-3} \text{ cm}^{-1}$ ) given in the HITRAN 2020 database.

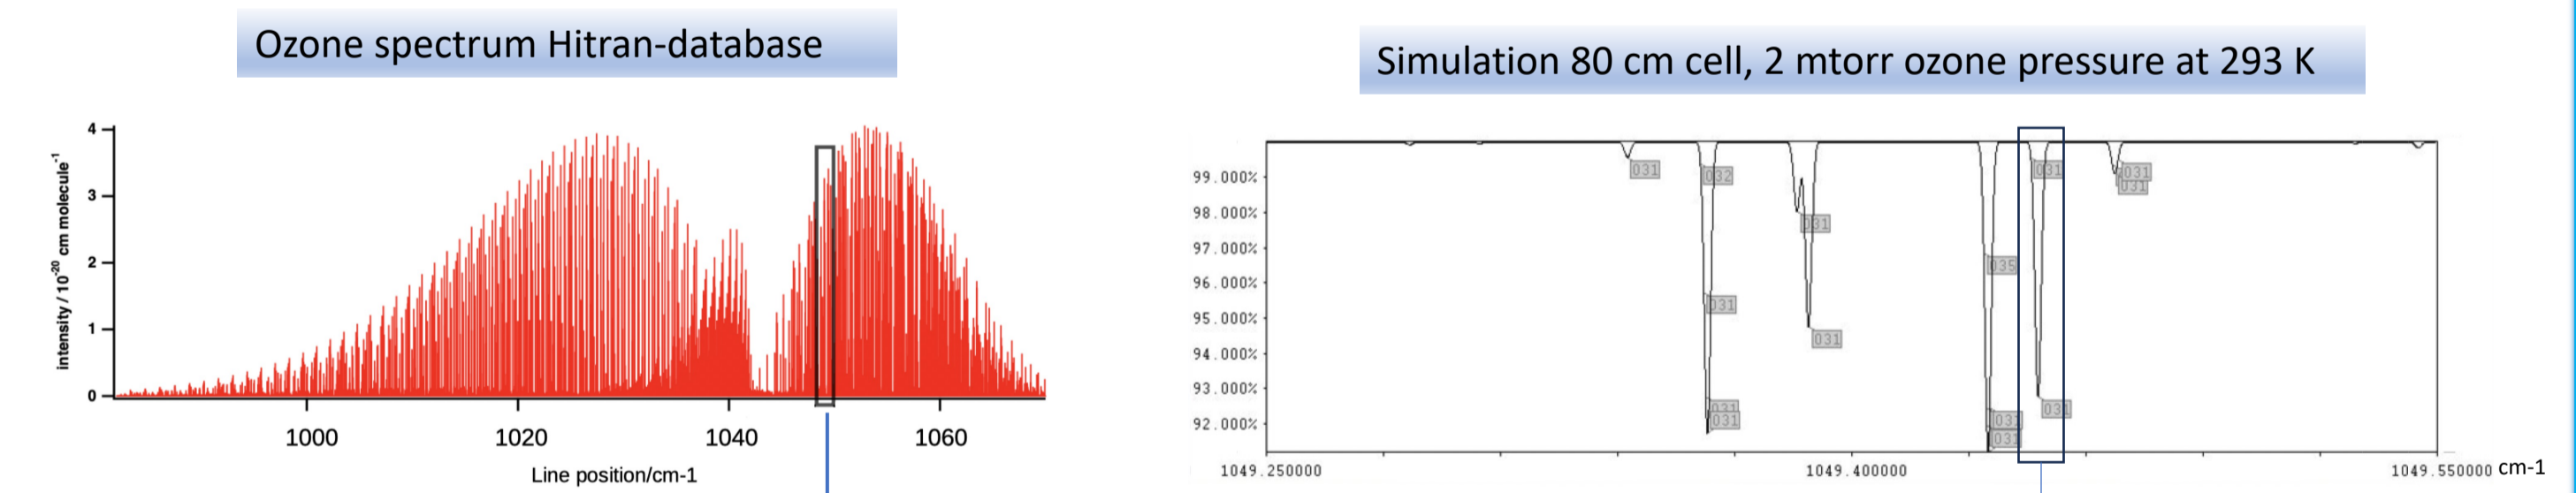


QCL down frequency sweep by current ramp

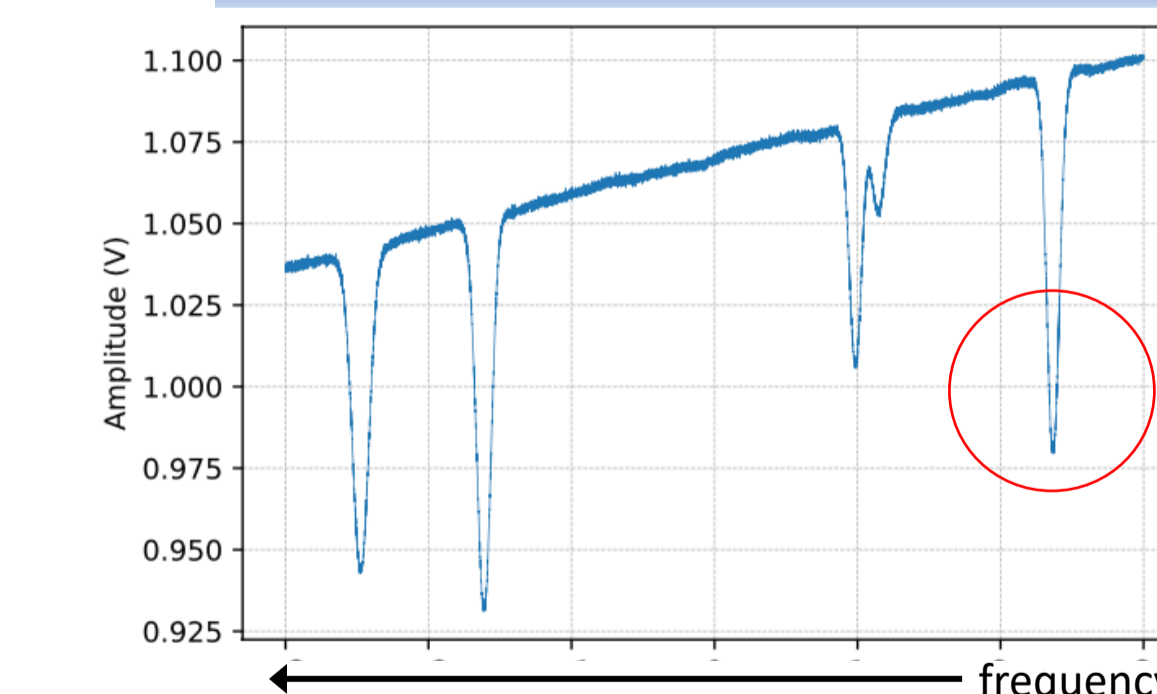


QCL frequency tuning by sweeping OFC repetition rate while locking QCL on OFC

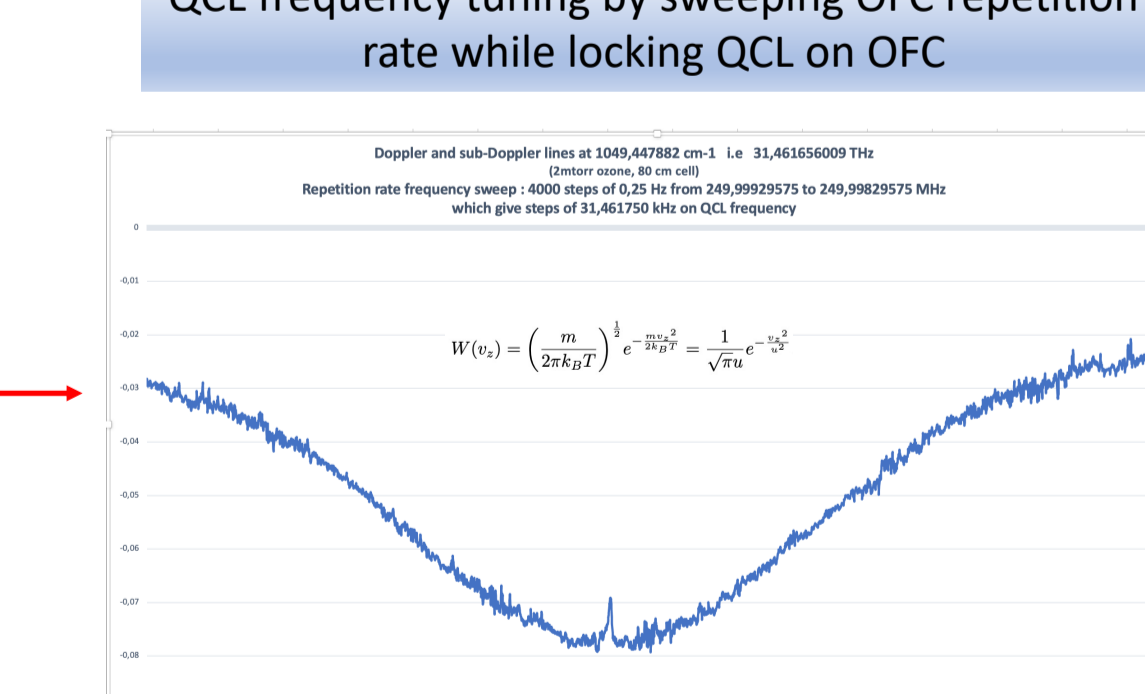

Second harmonic of the ozone Doppler free absorption line at 1049.447882  $\text{cm}^{-1}$ . Frequency offset by line position from Hitran data base.

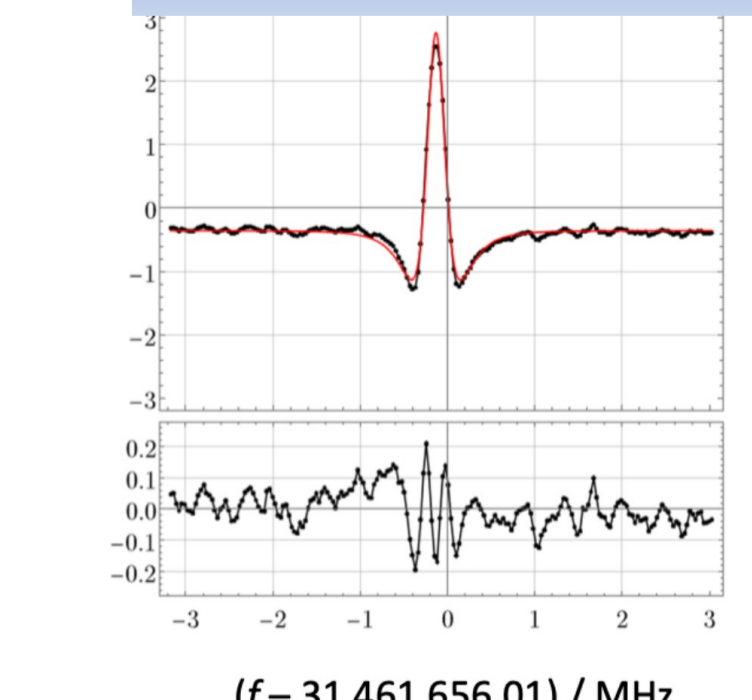

Doppler-free first harmonic modulation @ 10 kHz, 50 kHz deviation applied on the 50 MHz synthesizer

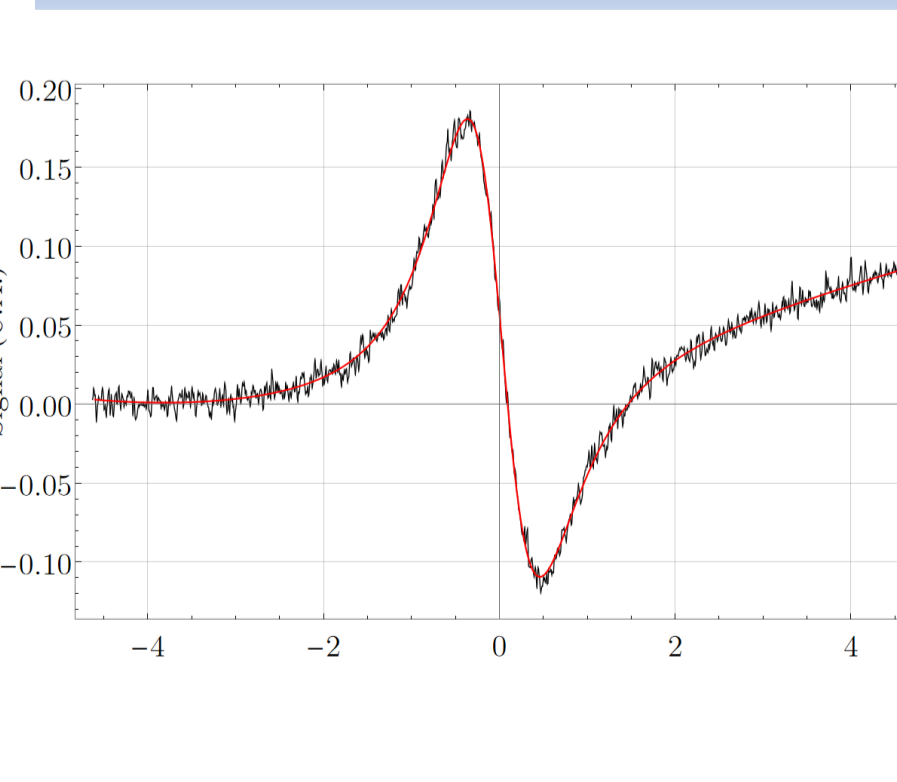

Conclusions

- Uncertainty (50 kHz) mainly limited by systematic effects
- Uncertainty almost three orders of magnitude smaller than in HITRAN (30 MHz).
- HITRAN2020 systematically shifted towards higher frequency, but very well within stated uncertainty.
- First absolute line position determination of the ozone main isotopologue  $^{16}\text{O}_3$  using sub-Doppler spectroscopy.
- Improvement towards  $< 4$  kHz uncertainty level is planned
- More systematic precision studies of line parameters (shape, position, pressure broadening and shift) are envisaged in the near future.

## References

1. N. Glatthor, T. von Clarmann, G. P. Stiller, M. Kiefer, A. Laeng, B. M. Dinelli, G. Wetzel, J. Orphal, Differences in ozone retrieval in MIPAS channels A and AB: a spectroscopic issue, Atmos. Meas. Tech. 11, 4707–4723 (2018).
2. M. Minissale, T. Zanon-Willette, P. Jeseck, C. Boursier, C. Janssen, First pressure shift measurement of ozone molecular lines at 9.54  $\mu\text{m}$  using a tunable quantum cascade laser. J. Molec. Spectrosc. 348, 103–113 (2018).
3. H. Tran, F. Rohart, C. Boone, M. Eremenko, F. Hase, P. Bernath, J.-M. Hartmann, Non-Voigt line-shape effects on retrievals of atmospheric ozone: Collisionally isolated lines, J. Quant. Spectrosc. Radiat. Transfer 111, 2012–2020 (2010).
4. B. Argence, B. Chanteau, O. Lopez, D. Nicolodi, M. Abgrall, C. Chardonnet, C. Daussey, B. Darquié, Y. Le Coq and A. Amy-Klein, Quantum cascade laser frequency stabilization at the sub-Hz level, Nature Photonics 2015
5. N. Cahuzac, B. Darquié, C. Janssen, Widely tuneable SI-traceable frequency comb-stabilized mid-infrared lasers for Earth system science and precise measurements in fundamental physics (project CNRS 80 PRIME) 2019.
6. E. Cantin et al., Current status of REFIMEVE fiber network in Paris urban area, Poster AG REFIMEVE 2023, Villetaneuse, France, 2023.

## Acknowledgment

This work has received funding from:  
FIRST-TF (ANR)  
REFIMEVE+ (ANR)  
CNRS (LEFE-CHAT, MITI PRIME80, INP) & SORBONNE-UNIVERSITE  
REGION ILE DE FRANCE

